



BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT

**METEOROLOGY AND MEASUREMENT DIVISION**

**2019 AIR MONITORING NETWORK PLAN**

July 1, 2019



***Duc Nguyen***  
***Jarrett Claiborne***  
***Richard Lam***  
***Caroline Normal***  
***Katherine Hoag***  
***Charles Knoderer***

Meteorology and Measurement Division 375 Beale St., Suite 600, San Francisco, CA 94105

This page intentionally left blank.

## TABLE OF CONTENTS

<b>Section</b>	<b>Page</b>
1..... INTRODUCTION.....	11
2..... OVERVIEW OF NETWORK OPERATION.....	11
2.1 ... Network Design .....	11
2.2 ... Minimum Monitoring Requirements .....	17
2.2.1 Minimum Monitoring Requirements for Ozone .....	20
2.2.2 Minimum Monitoring Requirements for PM <sub>2.5</sub> .....	24
2.2.3 Minimum Monitoring Requirements for PM <sub>10</sub> .....	30
2.2.4 Minimum Monitoring Requirements for Collocated PM <sub>10</sub> .....	34
2.2.5 Minimum Monitoring Requirements for SO <sub>2</sub> .....	34
2.2.6 Minimum Monitoring Requirements for NO <sub>2</sub> .....	38
2.2.7 Minimum Monitoring Requirements for CO .....	43
2.2.8 Minimum Monitoring Requirements for Lead.....	45
2.3 ... Modifications Made to Network in 2019.....	48
2.4 ... Proposed Modifications to Network in 2020–2021 .....	48
2.5 ... Removing a NAAQS Compliance Monitor .....	52
2.6 ... Data Submission Requirement.....	53
3..... SITE INFORMATION DEFINITIONS.....	54
4..... DETAILED STATION INFORMATION FOR SLAMS AND SPM SITES.....	59
4.1 ... Berkeley Aquatic Park (near-road) .....	60
4.2 ... Bethel Island.....	63
4.3 ... Concord .....	66
4.4 ... Crockett.....	70
4.5 ... Fairfield.....	72
4.6 ... Forest Knolls.....	74
4.7 ... Fort Cronkhite.....	76
4.8 ... Gilroy.....	78
4.9 ... Hayward.....	80
4.10. Laney College (near-road).....	82
4.11. Livermore.....	85
4.12. Los Gatos.....	89
4.13. Martinez.....	91
4.14. Napa Valley College .....	93
4.15. Oakland East .....	96
4.16. Oakland West .....	100

4.17. Palo Alto Airport.....	104
4.18. Pittsburg .....	106
4.19. Pleasanton (near-road).....	108
4.20. Point Richmond .....	110
4.21. Redwood City .....	112
4.22. Reid-Hillview Airport.....	115
4.23. Richmond 7 <sup>th</sup> .....	117
4.24. Rodeo .....	119
4.25. San Carlos Airport (II).....	121
4.26. San Francisco .....	123
4.27. San Jose – Jackson .....	127
4.28. San Jose – Knox (near-road).....	132
4.29. San Martin.....	135
4.30. San Pablo.....	138
4.31. San Rafael.....	142
4.32. San Ramon.....	146
4.33. Sebastopol.....	148
4.34. Vallejo.....	151
5. .... SPECIAL MONITORING PROGRAMS CONDUCTED IN 2018 .....	154
5.1 ... Meteorology Program .....	155
5.2 ... National Air Toxics Trends Station (NATTS) at San Jose.....	158
5.3 ... NCore Program .....	159
5.3.1 NCore Monitors .....	162
5.4 ... Photochemical Assessment Monitoring Stations (PAMS) .....	164
5.5 ... PM <sub>2.5</sub> Chemical Speciation Network (CSN) .....	170
5.5.1 BAAQMD Supplemental PM <sub>2.5</sub> Speciation Network Program.....	171
5.6 ... Toxics Program.....	174
5.6.1 Additional Toxics Monitoring at San Jose.....	178
APPENDIX A. OZONE MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD .....	180
APPENDIX B. APPENDIX B. PM <sub>10</sub> MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD .....	182
APPENDIX C. NO <sub>2</sub> MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD. .....	183
APPENDIX D. CO, NO <sub>2</sub> , AND PM <sub>2.5</sub> NEAR-ROAD MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD .....	185



APPENDIX E.	APPROVAL TO END MONITORING OF NO <sub>y</sub> AT THE SAN JOSE N CORE	
SITE	.....	188
APPENDIX F.	EPA'S APPROVAL TO END NO <sub>y</sub> MONITORING AT SAN JOSE N CORE	
SITE	.....	196
APPENDIX G.	REQUEST AND APPROVAL TO DISCONTINUE LEAD MONITORING AT	
SAN JOSE - JACKSON	.....	199
APPENDIX H.	NAPA SITE RELOCATION CORRESPONDENCE	.....204
APPENDIX I.	INITIAL PLAN FOR PAMS REQUIRED SITES	.....205
APPENDIX J.	SULFUR DIOXIDE DATA REQUIREMENTS RULE COMPLIANCE	
INFORMATION	.....	212

## LIST OF FIGURES

<b><u>Figure</u></b>		<b><u>Page</u></b>
Figure 2-1.	Map of Bay Area SLAMS and SPM Sites in 2019 .....	16
Figure 2-2. Area	Core Based Statistical Areas (CBSA) for the San Francisco Bay .....	19
Figure 2-3.	Ozone Monitoring in the San Francisco Bay Area in 2019.....	22
Figure 2-4.	PM <sub>2.5</sub> Monitoring in the San Francisco Bay Area in 2019.....	26
Figure 2-5.	PM <sub>10</sub> Monitoring in the San Francisco Bay Area in 2019.....	33
Figure 2-6.	SO <sub>2</sub> Monitoring in the San Francisco Bay Area in 2019 .....	37
Figure 2-7.	NO <sub>2</sub> Monitoring in the San Francisco Bay Area in 2019s .....	42
Figure 2-8.	CO Monitoring in the San Francisco Bay Area in 2019.....	44
Figure 2-9.	Lead Monitoring in the San Francisco Bay Area in 2019 .....	46
Figure 2-10.	Ozone Design Values from 2010-2019 .....	49
Figure 5-1.	Map of Air District Meteorological Monitoring Sites in 2019.....	157
Figure 5-2. station	Map showing area of Neighborhood Scale at the San Jose NCore .....	161
Figure 5-3.	Map of the two PAMS sites in the Livermore Valley .....	166

## LIST OF TABLES

<b><u>Table</u></b>	<b><u>Page</u></b>
Table 2-1. SLAMS Site Types and Appropriate Spatial Scales.....	14
Table 2-2. List of Monitoring Stations within the Air District in 2019 .....	14
Table 2-3. 2010 Census Population and 2018 Population Estimates for Bay Area CBSAs.....	18
Table 2-4. Minimum Monitoring Requirements for Ozone .....	21
Table 2-5. Minimum Monitoring Requirements for FRM/FEM PM <sub>2.5</sub> SLAMS.....	27
Table 2-6. Near-Road Monitoring for PM <sub>2.5</sub> .....	28
Table 2-7. Collocated PM <sub>2.5</sub> monitors for FEM networks .....	30
Table 2-8. Minimum Monitoring Requirements for SLAMS PM <sub>10</sub> .....	32
Table 2-9. Collocated PM <sub>10</sub> Monitoring in the Bay Area in 2019 .....	34
Table 2-10. Minimum Monitoring Requirements for SO <sub>2</sub> .....	36
Table 2-11. NO <sub>2</sub> Monitors at Various Spatial Scales .....	40
Table 2-12. Minimum Monitoring Requirements for NO <sub>2</sub> .....	41
Table 2-13. Minimum Monitoring Requirements for CO .....	43
Table 2-14. Source Oriented Lead Monitoring at Airports.....	47
Table 2-15. Collocated Source Oriented Lead Monitoring at Airports .....	47
Table 3-1. National Ambient Air Quality Standards (as of December 31, 2015) .....	54
Table 3-2. Monitor Information Definitions and EPA Air Monitoring Siting Criteria .....	55
Table 5-3. NCore Monitors .....	163
Table 5-4. Monitoring start date for PAMS sites .....	166

Table 5-5.	List of speciated hydrocarbons measured by Gas Chromatograph in 2019 .....	167
Table 5-6.	PM <sub>2.5</sub> Speciation Measurements at Air District Sites in 2019 .....	171
Table 5-7.	List of Toxic Compounds Measured by the Air District in 2019 .....	177

## Definition of Terms

1:1 .....	Particulate or toxic sample schedule that is taken every day
1:3 .....	Particulate or toxic sample schedule that is taken every 3 <sup>rd</sup> day
1:6 .....	Particulate or toxic sample schedule that is taken every 6 <sup>th</sup> day
1:12 .....	Particulate or toxic sample schedule that is taken every 12 <sup>th</sup> day
AADT .....	Annual Average Daily Traffic
AGL .....	Above Ground Level
APCD.....	Air Pollution Control District
AQMD.....	Air Quality Management District
AQS .....	Air Quality System; the EPA national air quality database
ARM .....	Approved Regional Method
Air District .....	Bay Area Air Quality Management District
BAM .....	Beta Attenuation Monitor, a type of continuous PM <sub>2.5</sub> monitor
BAAQMD .....	Bay Area Air Quality Management District
BC .....	Black Carbon
CARB .....	California Air Resources Board
CBSA .....	Core Based Statistical Area
CDP .....	Census Designated Place
CFR .....	Code of Federal Regulations
CO .....	Carbon Monoxide
CH <sub>4</sub> .....	Methane
CSN .....	Chemical Speciation Network
DOT .....	Department of Transportation
DRI .....	Desert Research Institute
EPA .....	U.S. Environmental Protection Agency
FE-AAADT .....	Fleet Equivalent Annual Average Daily Traffic
FEM .....	Federal Equivalent Method
FRM .....	Federal Reference Method
GC .....	Gas Chromatograph
GCMS.....	Gas Chromatograph Mass Spectrometer
GPS .....	Geographic Positioning System
HiVol .....	High Volume
HPLC.....	High Performance Liquid Chromatograph
H <sub>2</sub> S .....	Hydrogen Sulfide
ICPMS .....	Inductively Coupled Plasma Mass Spectrometry
IMPROVE .....	Interagency Monitoring of Protected Visual Environments
Maintenance Plan .....	A Plan submitted by states to EPA that outlines how the NAAQS will be maintained for a particular region.

## Definition of Terms (continued)

MBUAPCD .....	Monterey Bay Unified Air Pollution Control District
NAAQS .....	National Ambient Air Quality Standard
NATTS .....	National Air Toxics Trends Station
NCore .....	National Core (Monitoring Program)
NEI .....	National Emissions Inventory
NMHC .....	Non-methane Hydrocarbons
NO .....	Nitric Oxide
NO <sub>2</sub> .....	Nitrogen Dioxide
NO <sub>x</sub> .....	Oxides of Nitrogen
NO <sub>y</sub> .....	Total Reactive Nitrogen
NSR .....	New Source Review
O <sub>3</sub> .....	Ozone
PAMS .....	Photochemical Assessment Monitoring Stations
Pb .....	Lead
PPB .....	Parts per billion
PM .....	Particulate Matter
PM <sub>2.5</sub> .....	Particulates less than or equal to 2.5 microns in size
PM <sub>2.5F</sub> .....	PM <sub>2.5</sub> measured using a filter-based sampler
PM <sub>2.5C</sub> .....	PM <sub>2.5</sub> measured using a continuous monitor
PM <sub>10</sub> .....	Particulates less than or equal to 10 microns in size
PM <sub>10C</sub> .....	PM <sub>10</sub> measured using a continuous monitor
PM <sub>10-2.5</sub> .....	PM Coarse – PM less than or equal to 10 microns and greater than 2.5 microns in size
POC .....	Parameter Occurrence Code
PWEI .....	Population Weighted Emissions Index
SIP .....	State Implementation Plan – A Plan submitted by states to EPA that outlines how the NAAQS will be met for a particular region
SLAMS .....	State or Local Air Monitoring Station
SO <sub>2</sub> .....	Sulfur Dioxide
SPM .....	Special Purpose Monitor
STN .....	Speciation Trends Network
TAMS .....	Total Atmospheric Mercury
Toxics .....	Gaseous VOC toxic air contaminants (see Section 5.6)
TSP .....	Total Suspended Particulate
UFP .....	Ultrafine Particulate less than or equal to 0.1 microns
VOC .....	Volatile Organic Compound

## **1. INTRODUCTION**

This annual network plan for the Bay Area Air Quality Management District summarizes the air monitoring activities between January 1, 2018, and December 31, 2018. The detailed information about the instruments used at each air monitoring site pertains to the status as of December 31, 2018. There are also siting and local area descriptions for monitoring sites that operated in 2018 and for those that opened, or were planned to open, between January 1 and June 30, 2019.

## **2. OVERVIEW OF NETWORK OPERATION**

### **2.1 Network Design**

The Bay Area Air Quality Management District (Air District) is the public agency responsible for air quality management in the nine Bay Area counties: Alameda, Contra Costa, Marin, Napa, San Francisco, San Mateo, Santa Clara, southwestern Solano, and southern Sonoma. The Air District operates air monitoring stations in each of these nine counties. The Air District began measuring air quality in the San Francisco Bay Area in 1957. In 2019 there were 33 operational and two non-operational (airport lead) air monitoring stations within the Air District.

The Air District also performs air monitoring as part of several different programs. These include programs that the Air District has initiated, such as meteorological monitoring and the ambient toxics program, and programs required by the EPA. EPA programs currently include the National Core (NCore) program, the Photochemical Assessment Monitoring Stations (PAMS) program, and the PM<sub>2.5</sub> Chemical Speciation Network (CSN). Summaries of these programs can be found later in this report.

The San Francisco Bay Area contains more than 100 cities. Although resources do not allow for placement of air pollution monitors in every city, it can be demonstrated that air pollution levels, in the absence of significant local sources, are similar within each geographical region of the Bay Area. That is, cities within each of the major valleys of the Bay Area can have similar air quality levels. Consequently, a few sites can characterize an area. Generally, locations for permanent air monitoring sites are initially based on knowledge of population density, local wind patterns, topography, and sources of air emissions, while the final site selection is determined after analyzing preliminary air quality measurements collected from field studies, temporary monitoring studies, mobile monitoring data, and air quality modeling.

The monitoring objectives of the Air District's air monitoring network are:

- To provide air pollution data to the public in a timely manner.

- To support compliance with California and national ambient air quality standards.
- To support air pollution research studies.

To meet its monitoring objectives, the Air District collects ambient air data at locations with a variety of monitoring site types. These site types, as defined in 40 CFR Part 58, Appendix D, are listed below.

Highest concentration or maximum ozone concentration: Sites expected to have the highest concentration, even if populations are sparse in that area. High concentrations may be found close to major sources, or further downwind if pollutants are emitted from tall stacks. High concentrations also may be found at distant downwind locations when the pollutants such as ozone or secondary particulate matter are a result of chemical reactions in the atmosphere.

Population oriented: Sites established in areas with high population density to evaluate exposure to air pollution. In most cases, stations are located within the largest cities in each county. Because people spend more time at home than at work, air monitoring sites are generally located in residential areas rather than at downtown locations.

Source impact or source oriented: Sites in areas downwind of potential major sources of pollutants. The Air District operates source oriented SO<sub>2</sub> and H<sub>2</sub>S monitors near the five refineries that are potential sources of SO<sub>2</sub> and H<sub>2</sub>S: Chevron, Shell, Tesoro, Phillips 66, and Valero. Heavily trafficked roadways and the Port of Oakland are also significant sources of particulate matter, NO<sub>2</sub>, CO, and toxics. General aviation airports can be sources of lead because piston engine aircraft continue to use leaded fuel.

Upwind background: Sites in areas that have no significant emissions from mobile, area, or industrial sources. At these sites, the measured concentrations reflect the transported air quality levels from upwind areas.

General background: Where there are no significant emission sources upwind of a site, then the site is considered to be a general background site.

Regional transport: The Air District shares a common boundary with six other air districts: Monterey Bay Unified APCD, San Joaquin Valley APCD, Sacramento Metropolitan AQMD, Yolo-Solano AQMD, Lake County AQMD, and Northern Sonoma County APCD. When upwind areas have significant air pollution sources, pollutants may be transported into the Bay Area Air District and result in overall higher air pollution levels in the Bay Area. The Air District operates monitoring stations near the borders of the Air District to measure the air pollution concentrations transported into and out of



the Bay Area Air District.

Welfare-related impacts: Sites located to measure impacts on visibility, vegetative damage, or other welfare-based impacts.

Each site type is associated with a spatial scale. For example, a regional transport site is meant to represent air quality levels over a large area, while a highest concentration site may represent a spatial scale of no more than a few blocks in size. Spatial scales are defined in 40 CFR Part 58, Appendix D. They are: micro scale, having dimensions of several meters up to 100 m; middle scale, having dimensions of 100 m to 0.5 km; neighborhood scale, having dimensions of 0.5 km to 4.0 km; urban scale, having dimensions of 4 to 50 km; and regional scale, having dimensions of up to hundreds of km. Table 2-1 lists the appropriate scales for each site type.

Table 2-1. SLAMS Site Types and Appropriate Spatial Scales

Site Type	Appropriate Spatial Scale
Highest Concentration	Micro, middle, neighborhood
Population Oriented	Neighborhood, urban
Source Oriented	Micro, middle, neighborhood
General Background	Urban, regional
Regional Transport	Urban, regional

The spatial scale of a monitor must conform to established criteria for the distance from roadways, based on traffic volumes. There are different distance requirements for each pollutant, which can be found in 40 CFR Part 58, Appendix E. Table 2-2 lists the stations and the pollutants measured at each site and Figure 2-1 is a map of the monitoring sites in 2018.

Table 2-2. List of Monitoring Stations within the Air District in 2019

Site No.	Station Name	Pollutants Monitored <sup>1</sup>
1	Bethel Island	O <sub>3</sub> , NO <sub>x</sub> , SO <sub>2</sub> , CO, PM <sub>10</sub> , Toxics
2	Berkeley Aquatic Park (near-road)	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics, BC, UFP
3	Concord	O <sub>3</sub> , NO <sub>x</sub> , SO <sub>2</sub> , CO, PM <sub>10</sub> , PM <sub>2.5F</sub> , PM <sub>2.5C</sub> , Toxics
4	Crockett	SO <sub>2</sub> , Toxics
5	Fairfield	O <sub>3</sub>
6	Forest Knolls	BC
7	Fort Cronkhite	Toxics
8	Gilroy	O <sub>3</sub> , PM <sub>2.5C</sub>
9	Hayward	O <sub>3</sub>
10	Livermore	O <sub>3</sub> , NO <sub>x</sub> , PM <sub>2.5C</sub> , Speciated PM <sub>2.5</sub> , Toxics, BC, UFP
11	Los Gatos	O <sub>3</sub>
12	Martinez	SO <sub>2</sub> , Toxics
13	Napa Valley College	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>10</sub> , PM <sub>2.5C</sub> , Toxics
14	Oakland East	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics
15	Oakland - Laney College (near-road)	NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics, BC, UFP
16	Oakland West	O <sub>3</sub> , NO <sub>x</sub> , SO <sub>2</sub> , CO, PM <sub>2.5C</sub> , Speciated PM <sub>2.5</sub> , Toxics, BC
17	Palo Alto Airport	Lead (TSP) [not operational in 2019]
18	Pittsburg – Loveridge	Toxics, BC

<b>Site No.</b>	<b>Station Name</b>	<b>Pollutants Monitored<sup>1</sup></b>
19	Pleasanton – Owens Court (near-road)	NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics
20	Point Richmond	H <sub>2</sub> S
21	Redwood City	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics, UFP
22	Reid-Hillview Airport	Lead (TSP)
23	Richmond 7 <sup>th</sup>	SO <sub>2</sub> , H <sub>2</sub> S, Toxics
24	Rodeo	H <sub>2</sub> S
25	San Carlos Airport II	Lead (TSP) [not operational in 2019]
26	San Francisco	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>10</sub> , PM <sub>2.5C</sub> , Toxics
27	San Jose – Jackson	O <sub>3</sub> , NO <sub>x</sub> , NO <sub>y</sub> , SO <sub>2</sub> , CO, PM <sub>10</sub> , PM <sub>2.5F</sub> , PM <sub>2.5C</sub> , Speciated PM <sub>2.5</sub> , Toxics, Lead (PM <sub>10</sub> )
28	San Jose – Knox (near-road)	NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics, BC, UFP
29	San Martin	O <sub>3</sub>
30	San Pablo	O <sub>3</sub> , NO <sub>x</sub> , SO <sub>2</sub> , CO, PM <sub>10</sub> , PM <sub>2.5 C</sub> , Toxics, UFP
31	San Rafael	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>10</sub> , PM <sub>2.5C</sub> , Toxics
32	San Ramon	O <sub>3</sub> , NO <sub>x</sub>
33	Sebastopol	O <sub>3</sub> , NO <sub>x</sub> , CO, PM <sub>2.5C</sub> , Toxics, UFP
34	Vallejo	O <sub>3</sub> , NO <sub>x</sub> , SO <sub>2</sub> , CO, PM <sub>2.5C</sub> , Speciated PM <sub>2.5</sub> , Toxics

<sup>1</sup> See pages 9 and 10 for acronym definitions.



Figure 2-1. Map of Bay Area SLAMS and SPM Sites in 2019

## 2.2 Minimum Monitoring Requirements

The Air District met or exceeded all minimum monitoring requirements for most criteria pollutants in 2018. The three instances for which the Air District did not meet minimum monitoring requirements were due to circumstances beyond the Agency's control. These cases (near-road NO<sub>2</sub>, airport Pb, and PM<sub>10</sub>), and the Air District's ongoing efforts to resolve them, are discussed in the PM<sub>10</sub>, NO<sub>2</sub> and Pb portions of this section.

Smoke from wildfires occasionally significantly affects air quality within the Air District, especially in 2017 and 2018. The Air District has not yet requested that EPA exclude data affected by fires in 2017 or 2018 regulatory determinations; however, the resulting 2017-2019 design values for PM<sub>2.5</sub> are above the 24-hour PM<sub>2.5</sub> NAAQS for some CBSAs. The design values listed in the tables of this section have not been adjusted to remove data affected by exceptional events. The Air District may request at a future date that the affected data be excluded from regulatory determinations as exceptional events should NAAQS exceedances occur in subsequent design value years.

EPA minimum monitoring requirements are not based on the Air District boundary. Instead, they are based on Core Based Statistical Areas (CBSAs) or Metropolitan Statistical Areas (MSAs). CBSAs are either MSAs if the population is 50,000 or greater, or Micropolitan Statistical Areas ( $\mu$ SAs), if the population is less than 50,000. Since all our CBSAs are MSAs, not  $\mu$ SAs, the names and boundaries of the CBSAs and MSAs are identical. Because some CBSAs include multiple Air Districts, some monitors listed in the tables below are counted toward the minimum monitoring requirements even though the monitor is located in another air district. CBSA boundaries for the Bay Area are shown in Figure 2-2.

These minimum monitoring requirements are determined by evaluating certain data for the CBSA as described in 40 CFR 58 Appendix D. For population data, these are required to be based on the latest available census for O<sub>3</sub>, PM<sub>2.5</sub>, and NO<sub>2</sub>. SO<sub>2</sub> allows for population data to be based on either a census or population estimates, and CO and PM<sub>10</sub> requirements do not specify the data source. To use consistent populations for the CBSAs/MSAs within the Air District, the minimum monitoring requirements discussed below are based on the 2010 U.S. Census. The Air District does consider population estimates in our longer-term monitoring network planning, which is summarized in our Five-Year Network Assessments. Table 2-3 below lists the 2010 Census populations as well as 2018 estimated populations for each CBSA. While 2010 Census populations are

used to determine official requirements, the population estimates are used to evaluate potential future changes to these requirements, which are noted, as applicable.

Many minimum monitoring requirements are based on air quality data. The information for the highest site in a CBSA/MSA is given in the tables below and is based on 2017-2019 data. For a more complete overview of the air quality measured at the Air District sites including 2019 design values at all sites, please see the Annual Bay Area Air Quality Summary reports, posted online at <http://www.baaqmd.gov/about-air-quality/air-quality-summaries>.

Except where otherwise noted, each monitor meets the requirements of 40 CFR Part 58, appendices A, B, C, D, and E, where applicable.

Table 2-3. 2010 Census Population and 2018 Population Estimates for Bay Area CBSAs

<b>Core Based Statistical Area</b>	<b>2010 Census Population (April 1, 2010)</b>	<b>2019 Population Estimate (July 1, 2019)</b>
San Francisco-Oakland-Berkeley	4,335,391	4,731,803
San Jose-Sunnyvale-Santa Clara	1,836,911	1,990,660
Santa Rosa-Petaluma	483,878	494,336
Vallejo	413,344	447,643
Napa	136,484	137,744

Data source: <https://www.census.gov/data/datasets/time-series/demo/popest/2010s-total-metro-and-micro-statistical-areas.html>

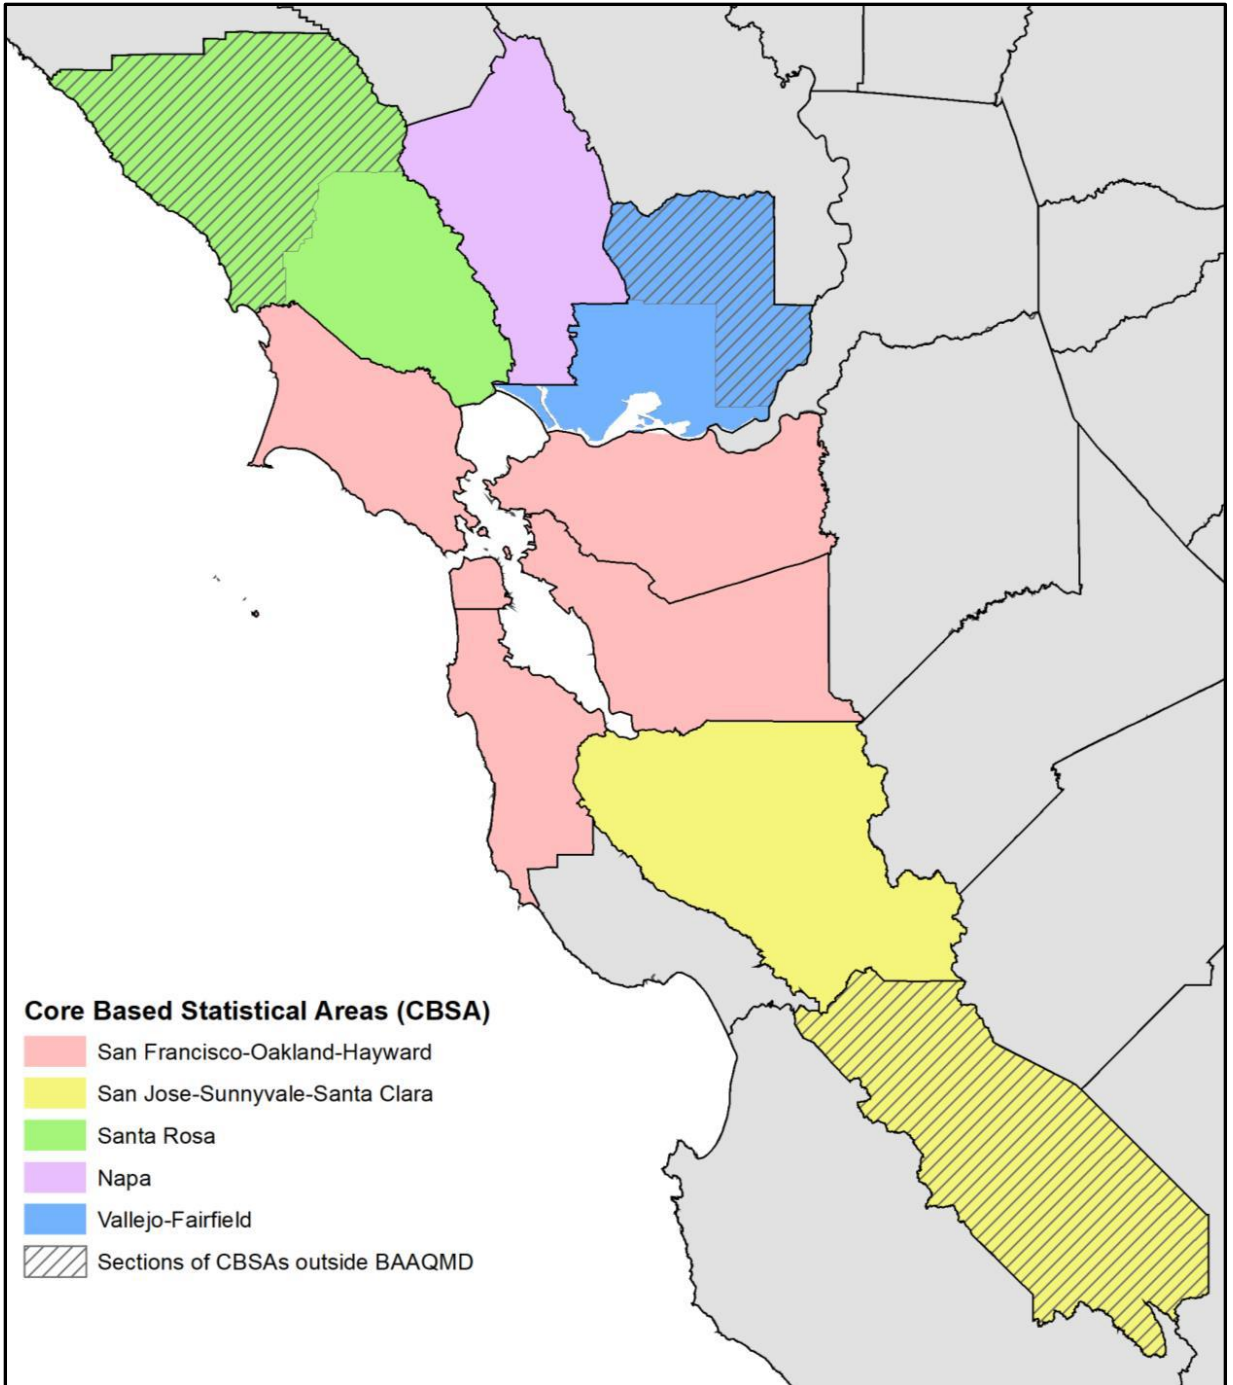


Figure 2-2. Core Based Statistical Areas (CBSA) for the San Francisco Bay Area

**Monitoring Agreements with Yolo/Solano AQMD and Northern Sonoma APCD**

The Bay Area network met all minimum monitoring requirements for all criteria pollutants in the Santa Rosa CBSA and the Vallejo–Fairfield CBSA, therefore, no interagency agreements were needed with these monitoring agencies. The Air District will

continue to assess the minimum monitoring requirements in the Five-Year Network Assessments and work with the other Air Districts to meet them.

### **Monitoring Agreements with Monterey Bay Unified APCD**

The Bay Area and Monterey Air Districts share minimum monitoring requirements for the San Jose–Sunnyvale–Santa Clara CBSA. This CBSA includes Santa Clara County (Bay Area) and San Benito County (Monterey). Shared pollutant monitoring agreements include O<sub>3</sub>, PM<sub>2.5</sub>, PM<sub>10</sub>, and near-road NO<sub>2</sub>, CO, and PM<sub>2.5</sub>. Within its own network, the Bay Area Air District meets minimum monitoring requirements for O<sub>3</sub>, PM<sub>2.5</sub>, and near-road NO<sub>2</sub>, CO, and PM<sub>2.5</sub>. PM<sub>10</sub> is the only pollutant that the Bay Area does not meet the minimum requirements on its own, and therefore has a monitoring agreement with Monterey Bay for PM<sub>10</sub>. Monterey Bay needs agreements for O<sub>3</sub>, PM<sub>2.5</sub>, and near-road NO<sub>2</sub>, CO, and PM<sub>2.5</sub> monitoring. Existing agreements are in Appendix A (O<sub>3</sub>), Appendix B (PM<sub>10</sub>), Appendix C (NO<sub>2</sub>), and Appendix D (near-road CO, NO<sub>2</sub>, and PM<sub>2.5</sub>).

#### **2.2.1 Minimum Monitoring Requirements for Ozone**

The number of required ozone (O<sub>3</sub>) monitors in each MSA is determined by the MSA population and design value, as specified in Table D-2 of 40 CFR Part 58, Appendix D. O<sub>3</sub> design values are calculated for each site according to 40 CFR Part 50, Appendix I and are compared to the National Ambient Air Quality Standard (NAAQS) to determine the attainment status of an area.

The 2019 Air District monitoring network for O<sub>3</sub> (Figure 2-3) meets or surpasses the O<sub>3</sub> minimum monitoring requirements (Table 2-4). Therefore, no monitoring agreement is needed between the Bay Area Air Quality Management District and any other air district to comply with the minimum monitoring requirement for O<sub>3</sub>.

The Bay Area was designated nonattainment for both the 1997 and the 2008 8-hour O<sub>3</sub> NAAQS, with area classifications of “marginal.” Updated design values based on the last three years of data (2017-2019) show that O<sub>3</sub> concentrations are now in attainment of both these NAAQS; however, the Bay Area will continue to be designated as nonattainment until the Air District submits a redesignation request and a maintenance plan to the EPA and the EPA approves the redesignation and maintenance plan. No additional monitors are required in the State Implementation Plan (SIP) or Maintenance Plan for O<sub>3</sub>. On April 30, 2018, EPA designated the Bay Area nonattainment for the 2015 8-hour O<sub>3</sub> NAAQS, with a classification of marginal.



Table 2-4. Minimum Monitoring Requirements for Ozone

MSA	County or Counties	Population 2010 Census	2019 8-hour Design Value (ppb)	Design Value Site and AQS ID	Number of SLAMS		
					Required	Active	Additional Needed
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	73	Livermore 06-001- 0007	3	7	0
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	65	San Martin 06-085-2006	2	6 <sup>b</sup>	0
Santa Rosa-Petaluma	Sonoma	483,878	57	Healdsburg 06-097-1003	1	2 <sup>c</sup>	0
Vallejo	Solano	413,344	64	Vacaville 06-095-3003	2	3 <sup>d</sup>	0
Napa	Napa	136,484	59	Napa Valley College 06-055-0004	0 <sup>e</sup>	1	0

<sup>a</sup> Design values are calculated at each monitoring site by taking the 3-year mean (2017-2019) of the 4th highest 8-hour concentration. The design values shown for each MSA in this table are the highest design value of monitors in the MSA. Design values at or below the 0.070 ppm meet the 8-Hour O<sub>3</sub> NAAQS. No fire-affected data have been excluded from this calculation.

<sup>b</sup> Two of the six monitors are not in the BAAQMD. They are in Hollister and Pinnacles National Park which are in the Monterey Bay Unified APCD. The Pinnacles monitor is part of the CASTNET program and was designated SLAMS in 2010 by the EPA.

<sup>c</sup> One of the two monitors is not in the BAAQMD. It is in Healdsburg which is in the Northern Sonoma County APCD.

<sup>d</sup> One of the three monitors is not in the BAAQMD. It is in Vacaville which is in the Yolo-Solano AQMD.

<sup>e</sup> EPA Region 9 analysis of the Napa-Jefferson Street site (06-055-0003) showed that the design value would increase by 2 ppb if this site was located at a neighborhood scale instead of middle scale site. However, the required number of SLAMS monitors would be unchanged (one) for the Napa MSA. The Napa-Jefferson Street site (06-055-0003) was relocated to the Napa Valley College site (06-055-0004), a neighborhood scale site, on April 1, 2018. The site relocation was approved by EPA, and data from both sites were combined for the purpose to computing the 8-hour design value as shown above.

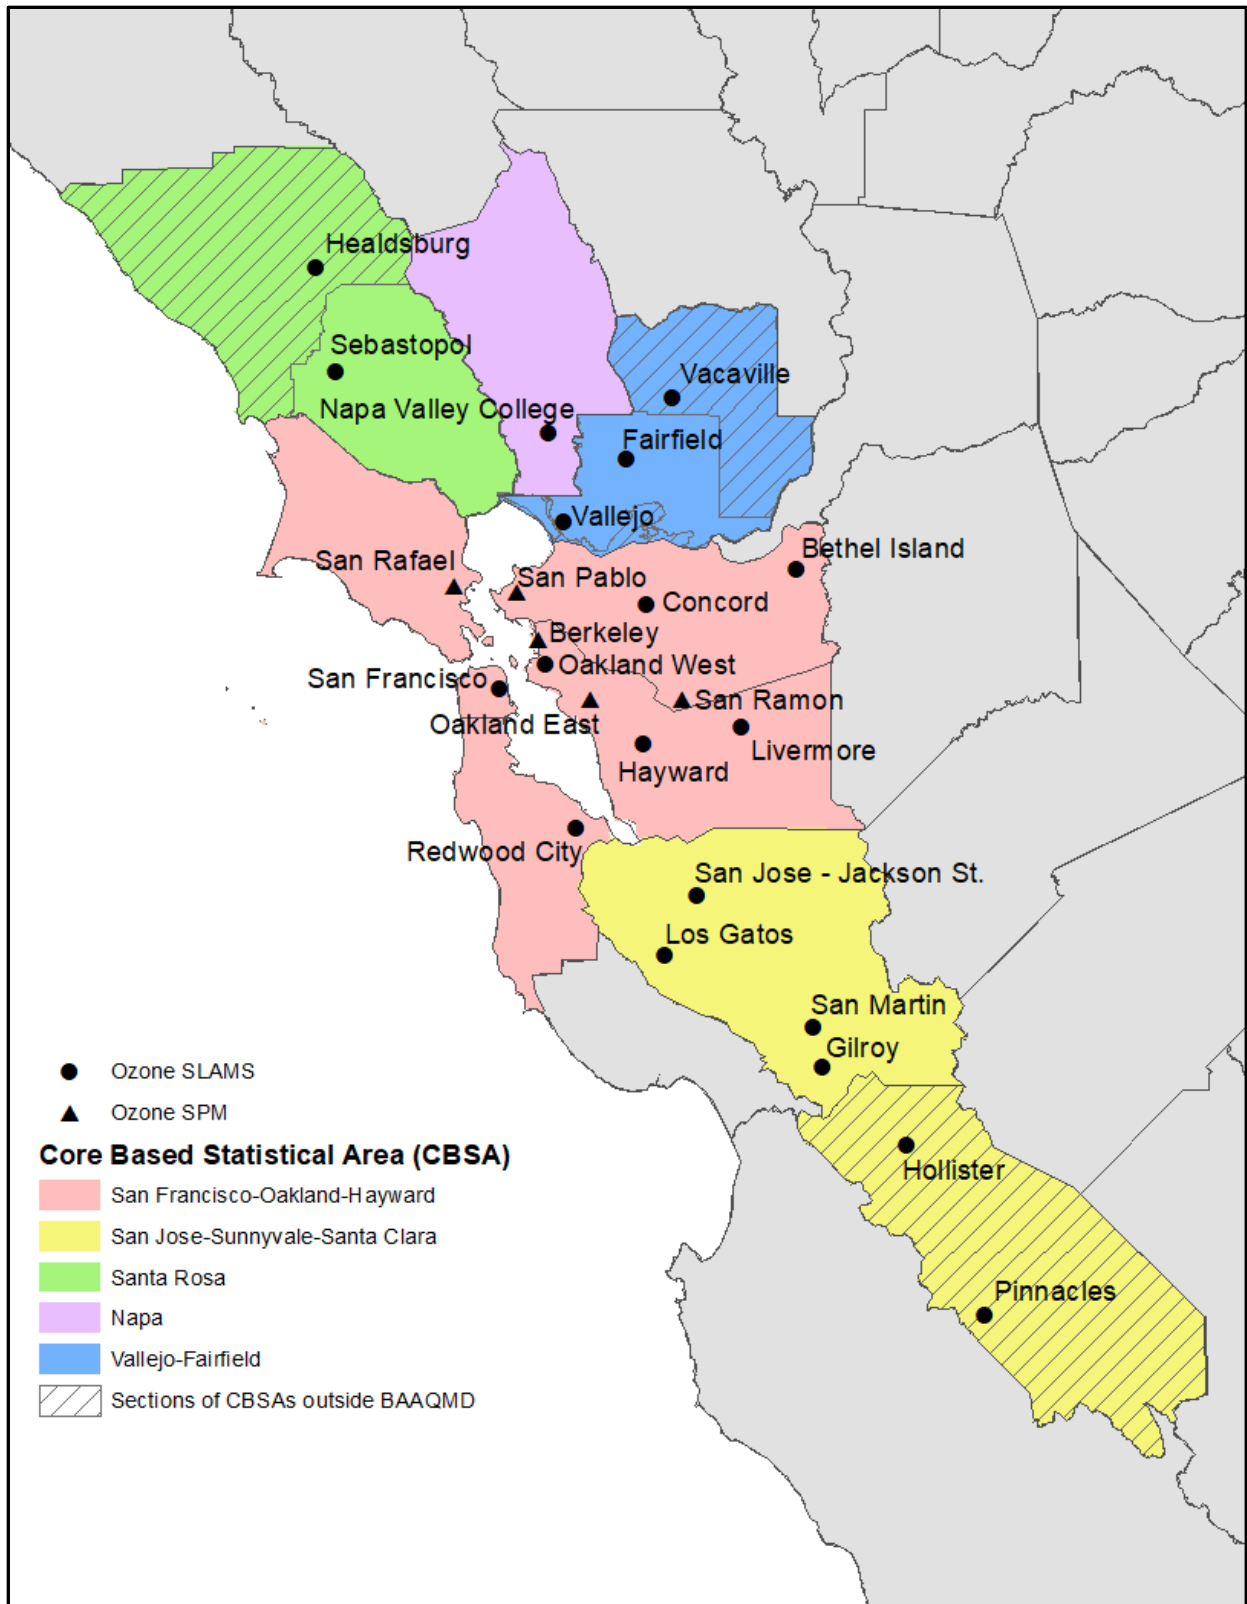


Figure 2-3. Ozone Monitoring in the San Francisco Bay Area in 2019

## **Ozone Special Purpose Monitors**

There are four O<sub>3</sub> monitors (San Rafael, San Pablo, Berkeley-Aquatic Park, and Oakland East) that are too close to a roadway to meet the siting requirements of 40 CFR 58 Appendix E. The proximity of these sites to the roadway may bias the O<sub>3</sub> concentrations lower than is representative. Therefore, these monitors are designated as special purpose monitors (SPMs) and as such are not counted towards minimum monitoring requirements.

However, in other ways these monitors are representative of population exposure in the near-road environment, and meet the requirements of 40 CFR 58 Appendix A. They are, therefore, considered to be comparable to the NAAQS, in that a violation of the NAAQS measured at one of these sites is still valid. Section 16 of EPA's Near-Road NO<sub>2</sub> Monitoring Technical Assistance Document provides a discussion of O<sub>3</sub> monitoring at near-road sites: <https://www3.epa.gov/ttnamti1/nearroad.html>.

The San Ramon O<sub>3</sub> SPM meets the requirements of 40 CFR 58 Appendices E and A, and is operated seasonally (see below). It is considered comparable to the NAAQS since it has been operating for over 24 months, but it is not counted towards minimum O<sub>3</sub> monitoring requirements.

EPA noted in their 2018 TSA that the Hayward O<sub>3</sub> monitor also does not meet 40 CFR 58 Appendix E siting requirements and noted that it should, therefore be classified as an SPM. The Air District is requesting that EPA approve the change in monitoring type of this monitor from a SLAMS to an SPM as suggested (see Section 2.3). If approved as an SPM, the Hayward O<sub>3</sub> monitor will not be counted towards minimum monitoring requirements in future years, however, the San Francisco-Oakland-Berkeley CBSA will still meet minimum monitoring requirements.

## **Napa Ozone Spatial Scale, Waiver Request**

The Napa-Jefferson Street O<sub>3</sub> monitor (06-055-0003) was classified as middle scale based on the nearby traffic count and distance between the monitor and the roadway (per 40 CFR Part 58). An Air District analysis concluded that recorded O<sub>3</sub> concentrations at Napa were not appreciably affected by NO<sub>2</sub> emissions from the nearest roadway. Subsequently, the Air District applied for a waiver from EPA Region 9 for this monitor to be classified as a SLAMS and be counted toward the requirement for a maximum concentration O<sub>3</sub> site in the Napa MSA despite not meeting the roadway distance requirement for a neighborhood scale site.

In response to this request, EPA used a conservative approach to estimate how much O<sub>3</sub> measured at the Napa-Jefferson Street site was decreased due to NO<sub>2</sub> emitted from nearby roadways. Based on this analysis, EPA concluded that the Napa O<sub>3</sub> design value may have been 2 ppb higher if the monitor had been far enough away from the roadway to meet EPA siting criteria. Therefore, EPA Region 9 granted the waiver, applying it to all future years as long as the site's design value was not within 5 ppb of any applicable NAAQS. As described in last year's Plan, the data collected at the Napa – Jefferson Street site through the site's closure on March 31, 2018 is low enough so that this waiver applies through the end of that monitors data record.

The Napa CBSA monitoring site relocated to the Napa Valley College site and began operations as a SLAMS on April 1, 2018. This site meets neighborhood scale representativeness and the requirements of appendices A, B, C, D, and E. Therefore, there is no need for a waiver for the Napa MSA O<sub>3</sub> monitoring requirements to be met this year or future years.

## **2.2.2 Minimum Monitoring Requirements for PM<sub>2.5</sub>**

The number of required PM<sub>2.5</sub> monitors in each MSA is determined by the MSA population and design value, as specified in Table D-5 of Appendix D to 40 CFR Part 58. The Air District's network of PM<sub>2.5</sub> SLAMS and SPMs are shown in Figure 2-4. Table 2-5 shows that the PM<sub>2.5</sub> minimum requirements for SLAMS monitoring were met in 2019.

In 2019, every PM<sub>2.5</sub> monitor in the network was a Federal Reference Method (FRM) or Federal Equivalent Method (FEM), and the primary monitor at every site was a continuous FEM. While the near-road sites at Oakland-Laney College, Berkeley Aquatic Park, Pleasanton, and San Jose-Knox are considered micro-scale because of their distance to roadways, they are considered area-wide sites since they represent many similar locations throughout their MSAs (see 40 CFR Part 58, Appendix D §4.7.1(b)). The Pleasanton site is designated an SPM and meets the requirements of 40 CFR 58 Appendices A, B, C, D, and E. As an SPM, it is not counted towards minimum monitoring requirements.

The Air District does not need any monitoring agreements with Northern Sonoma County APCD, Monterey Bay Unified ACPD or Yolo-Solano AQMD for PM<sub>2.5</sub> because the Bay Area network meets the requirements for those MSAs shared with those Air Districts. No additional monitors are required by State Implementation Plans or Maintenance Plans.

In addition to the requirement for a minimum number of PM<sub>2.5</sub> SLAMS, EPA requires that a certain number of sites operate continuous PM<sub>2.5</sub> monitors (40 CFR Part 58, Appendix D

§4.7.2). Currently, all the primary PM<sub>2.5</sub> monitors in the Air District network are continuous FEMs. Therefore, the requirement to operate continuous PM<sub>2.5</sub> monitors equal to at least one-half (rounding up) the number of PM<sub>2.5</sub> SLAMS monitors is met.

The PM<sub>2.5</sub> network design requirements and the minimum number of near-road PM<sub>2.5</sub> monitors in the PQAQ (40 CFR Part 58, Appendix D §4.7.1(b)(2)) and the QA requirements for the collocation of PM<sub>2.5</sub> monitors (40 CFR Part 58, Appendix A §3.2.5) are discussed below.

### **State Implementation Plan (SIP) Requirements**

EPA designated the Bay Area as nonattainment of the 2006 24-hour PM<sub>2.5</sub> NAAQS on October 8, 2009. The effective date of the designation was December 14, 2009, and the Air District had three years to develop a State Implementation Plan (SIP) to demonstrate that the Bay Area will achieve the revised standard by the attainment date of December 14, 2014. However, in October 2012, EPA proposed to suspend some of the SIP requirements after making a Clean Data Determination, as described below.

On December 18, 2014, EPA designated the Bay Area as unclassifiable/attainment for the 2012 Annual PM<sub>2.5</sub> NAAQS. Areas designated as unclassifiable/attainment are not required to submit a SIP.

### **Clean Data Determination by U.S. EPA**

On January 9, 2013, EPA issued a final rule determining that the Bay Area is attaining the 2006 24-hour PM<sub>2.5</sub> NAAQS, suspending key SIP requirements as long as monitoring data continues to show that the Bay Area attains the PM<sub>2.5</sub> standard.

Although most SIP requirements are suspended, the Bay Area was still required to prepare and submit an abbreviated SIP to address the required elements, including:

- An emission inventory for primary PM<sub>2.5</sub>, as well as precursor pollutants that contribute to formation of secondary PM; and
- Amendments to the Air District's New Source Review (NSR) to address PM<sub>2.5</sub> (as well as other revisions). Amendments to the NSR were adopted by the Air District's Board of Directors on December 19, 2012.

The Bay Area will continue to be designated as nonattainment for the 2006 24-hour PM<sub>2.5</sub> NAAQS until the Air District elects to submit, and the EPA approves, a redesignation request and maintenance plan.

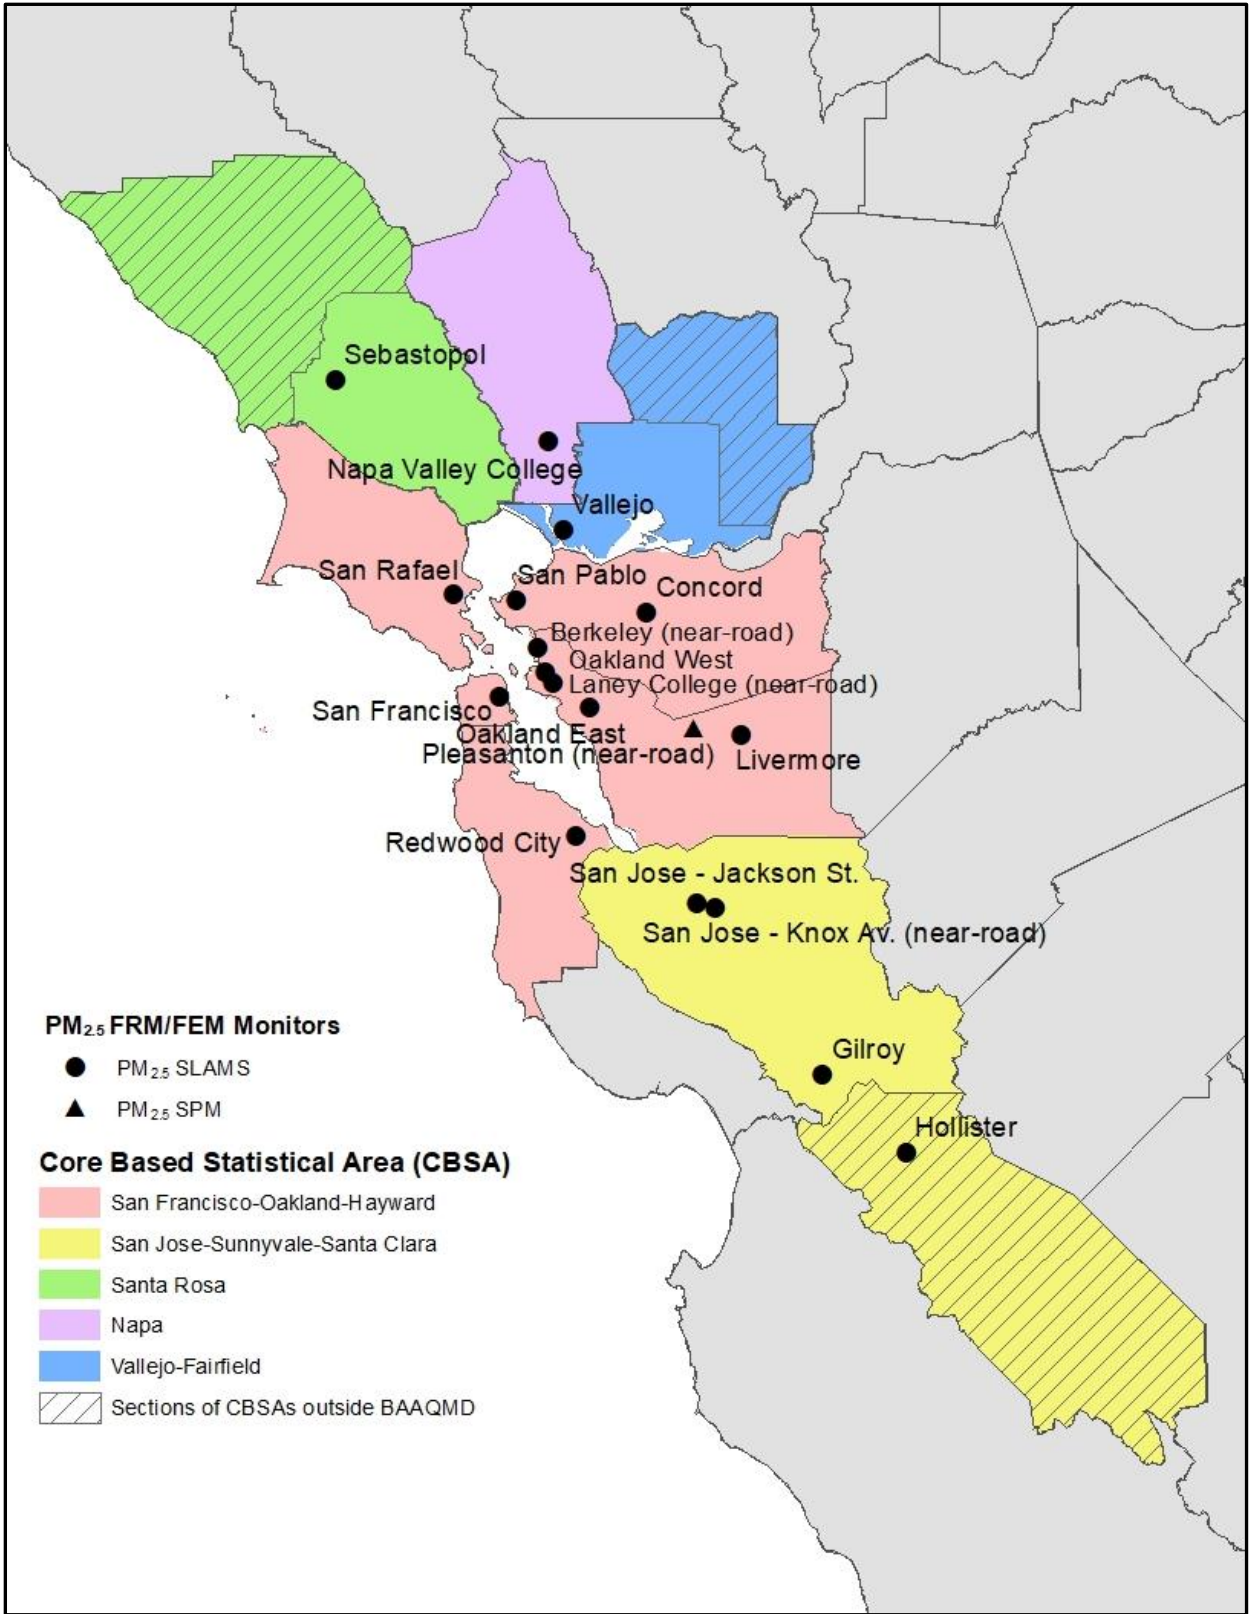


Figure 2-4. PM<sub>2.5</sub> Monitoring in the San Francisco Bay Area in 2019

Table 2-5. Minimum Monitoring Requirements for FRM/FEM PM<sub>2.5</sub> SLAMS

MSA	County or Counties	Population <sup>a</sup> 2010 Census	2019 Annual Design Value <sup>b</sup> (µg/m <sup>3</sup> ) Design Value Site (AQS ID)	Number of SLAMS		
			2019 Daily Design Value <sup>c</sup> (µg/m <sup>3</sup> ) Design Value Site (AQS ID)	Required	Active	Additional Needed
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	11.7 Oakland West (06-001-0011) 45 Oakland West and Laney College <sup>d</sup> (06-001-0011 and 06-001-0012)	3	10 <sup>e</sup>	0
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	10.5 San Jose-Jackson (08-085-0005) 43 San Jose-Jackson and San Jose-Knox Ave <sup>d</sup> (06-085-0005 and 06-085-0006)	3	4 <sup>f</sup>	0
Santa Rosa-Petaluma	Sonoma	483,878	7.4 Sebastopol (06-097-0004) 35 Sebastopol (06-097-0004)	1	1	0
Vallejo	Solano	413,344	11.2 Vallejo (06-095-0004) 48 Vallejo (06-095-0004)	1	1	0
Napa	Napa	136,484	10.4 <sup>g</sup> Napa and Napa Valley College (06-005-0003 and 06-055-0004) 46 <sup>g</sup> Napa and Napa Valley College (06-005-0003 and 06-055-0004)	1	1	0

<sup>a</sup> Per 40 CFR Part 58 Appendix D, Table D-5 footnote 2, minimum monitoring requirements for PM<sub>2.5</sub> are based on MSA populations from the latest available census figures.

<sup>b</sup> Annual design values are calculated at each monitoring site by taking the 3-year mean (2017-2019) of the annual averages for each site. The design values shown for each MSA in this table are the highest design value of monitors in the MSA. Design values at or below 12.0 µg/m<sup>3</sup> indicate the area meets the 2012 Annual PM<sub>2.5</sub> NAAQS. Listed design values include data affected by wildfire emissions.

<sup>c</sup> Daily design values are calculated by taking the 3-year mean (2017-2019) of the 98th percentiles for each site. The design values shown for each MSA in this table are the highest design value of monitors in the MSA. Design values at or below 35 µg/m<sup>3</sup> indicate the area meets the 2006 24-hour PM<sub>2.5</sub> NAAQS. Listed design values include data affected by wildfire emissions.

<sup>d</sup> These two sites had the same 2019 Daily Design Value.

## **Near-road PM<sub>2.5</sub> Sites**

Along with the 2012 PM<sub>2.5</sub> NAAQS revision, EPA also revised the PM<sub>2.5</sub> network design criteria to require at least one PM<sub>2.5</sub> monitor at near-road sites in CBSAs with populations of 1 million or greater (40 CFR 58, Appendix D §3.7.1 (b)(2)). The minimum monitoring requirements are met and shown in Table 2-6.

Table 2-6. Near-Road Monitoring for PM<sub>2.5</sub>

Metropolitan Statistical Area	County or Counties	Population <sup>a</sup> 2010 Census	Number of Near-road PM <sub>2.5</sub> SLAMS	
			Required	Active
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	1	2 <sup>a</sup>
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	1	1
Santa Rosa-Petaluma	Sonoma	483,878	0	0
Vallejo	Solano	413,344	0	0
Napa	Napa	136,484	0	0

<sup>a</sup> The Pleasanton-Owens Ct. site meets siting for a near-road monitoring objective. However, the PM<sub>2.5</sub> monitor at that site that is an SPM, and as such, is not counted toward fulfilling the requirements of 40 CFR 58, Appendix D §3.7.1 (b)(2).

## **Area of Expected Maximum Concentration**

Network design requirements for PM<sub>2.5</sub> require sites in each MSA located in areas of expected maximum concentrations (40 CFR 58 Appendix D). The Air District siting for PM<sub>2.5</sub> takes into account the potential effect on air quality from many PM<sub>2.5</sub> source types, including stationary and area sources, roadways, residential wood burning, and agriculture. The primary objective of these maximum concentration SLAMS is to determine compliance with the PM<sub>2.5</sub> NAAQS. Because the NAAQS are based on annual averages or the 98th percentile daily average PM<sub>2.5</sub> concentrations, these sites should be located where the annual average or 98th percentile concentration are expected to be highest most years, even though another location may experience higher concentrations on a specific day. Also, the maximum concentration site should characterize sources that could be important on a variety of days.



EPA determined that the current PM<sub>2.5</sub> monitoring network in the Bay Area meets this requirement. Air District regularly evaluates the amount and distribution of PM<sub>2.5</sub> (direct and precursor) source emissions through emissions inventory and modeling work for other programs and uses this work to assess the effectiveness of the ambient monitoring network for each 5-Year Network Assessment.

### **Regional Background and Transport Sites**

Every state is required to operate at least one regional transport site and one regional background site (40 CFR 58, Appendix D §4.7.3). While some of sites like Vallejo, Livermore, and others at times measure transport between the Bay Area and the Central Valley, or relatively clean air off the ocean, they are not considered regional background or transport sites for the purpose of this requirement. Since these are state-wide requirements, more information about transport and background sites in California can be found in the California Air Resource Board's Annual Monitoring Network Report, found at <http://www.arb.ca.gov/aqd/aqmoninca.htm>.

### **PM<sub>2.5</sub> Filter Analysis for Other Air Districts and PQAO Responsibility**

Because the Air District has a fully staffed professional Laboratory Services Section, PM<sub>2.5</sub> filter samples collected by the North Coast AQMD and Monterey Bay Unified APCD are weighed by staff at the Air District's laboratory. The Bay Area Air District, however, is not the Primary Quality Assurance Organization (PQAO) for these samples. Therefore, the PM<sub>2.5</sub> concentrations are sent back to the collecting agencies for their review, data validation, and certification. The Bay Area Air Quality Management District is the certifying agency for samples collected within the Bay Area only.

### **Minimum Monitoring Requirements for Collocated PM<sub>2.5</sub>**

In 2019, the Bay Area operated 17 primary PM<sub>2.5</sub> monitors (SLAMS and SPMs); these primary monitors were all MetOne BAM continuous FEMs (method 170). EPA requires collocation at 15% of the sites (round up) which equates to three collocated monitors, the first and third collocated monitors must be an FRM and the second must be the same FEM method as the primary monitor (see 40 CFR 58, Appendix A §3.2.3). In 2019, the Bay Area had three sites with collocated PM<sub>2.5</sub> monitors, San Jose-Jackson and Concord with FEM-primary and FRM-collocated, and Vallejo with a FEM/FEM primary/collocated pair, as shown in Table 2-7 below.

Table 2-7. Collocated PM<sub>2.5</sub> monitors for FEM networks

Method Code	# Primary Monitors	# Required Collocated Monitors	# Active Collocated FRM Monitors	# Active Collocated FEM Monitors (same method as primary)
170	17	3	2 San Jose-Jackson and Concord	1 Vallejo

Historically, the San Jose-Jackson, Concord and Vallejo sites have had some of the highest design PM<sub>2.5</sub> values in the Bay Area, which is why these sites were selected for collocated monitoring. The Bay Area did not meet the collocated PM<sub>2.5</sub> requirement in 2018. The Air District installed an FRM at Concord on February 8, 2019 to meet this requirement.

### 2.2.3 Minimum Monitoring Requirements for PM<sub>10</sub>

The number of required PM<sub>10</sub> monitors in each MSA is specified in Table D-4 of Appendix D to 40 CFR Part 58. To meet the requirements, a monitoring agreement is needed between the Air District and the Monterey Bay Unified APCD for the San Jose – Sunnyvale – Santa Clara MSA. The Bay Area operates one monitor in Santa Clara County and Monterey Bay operates one monitor in San Benito County. The monitoring agreement is presented in Appendix B.

There are no monitoring agreements with either the Northern Sonoma APCD or the Yolo-Solano AQMD because neither the Santa Rosa MSA nor the Vallejo MSA are required to have any PM<sub>10</sub> monitors. No additional monitors are required for the State Implementation Plan or Maintenance Plan because the Bay Area has never been designated as nonattainment for PM<sub>10</sub>.

The maximum concentration in 2019 at the Hollister site in the San Jose – Sunnyvale – Santa Clara MSA was affected by a rare high pressure event that brought air into the basin from the San Joaquin Valley. This unusual event caused the highest day for PM<sub>10</sub> at that site in at least eight years. The next highest values from 2013-2019 at that site are as follows: 96 µg/m<sup>3</sup> in 2019, 85 µg/m<sup>3</sup> in 2013, 80 µg/m<sup>3</sup> in 2018, and 79 µg/m<sup>3</sup> in 2017. During 2014-2016, the site did not have any days above 50 µg/m<sup>3</sup>. Additionally, this late October 2019 event did not have as significant an effect on Santa Clara County, where the maximum concentration during this time was 75 µg/m<sup>3</sup>. Santa Clara is the more populous part of the San Jose – Sunnyvale – Santa Clara MSA by far, and existing monitoring meets the needs of the local air districts and the communities since the Hollister site already captures the relevant information for this type of event. The Air

District will continue to work with Monterey Bay Unified APCD to assess the adequacy of the PM<sub>10</sub> network in the San Jose-Sunnyvale-Santa Clara CBSA in each 5-Year Network Assessment, evaluating the need for additional monitoring taking available resources for the construction and operation of new sites into consideration. The Air District is committed to working with EPA, CARB, and other local air districts to ensure that monitoring levels continue to protect public health and safety.

### **PM<sub>10</sub> Special Purpose Monitors**

Special purpose PM<sub>10</sub> monitoring at Bethel Island, Concord, and San Francisco is conducted at a sampling frequency of 1:12. These SPM monitors meet 40 CFR Appendices E and A, and are considered NAAQS comparable since they could show a valid violation of the NAAQS, but are not counted toward meeting the minimum monitoring requirements.

Table 2-8 and Figure 2-5 show the required PM<sub>10</sub> monitors, the active SLAMS counted toward those requirements, and the locations of all the PM<sub>10</sub> SLAMS and SPMs in the PQAQ.

Table 2-8. Minimum Monitoring Requirements for SLAMS PM<sub>10</sub>

MSA	County or Counties	Population 2010 Census	Highest 24-Hour Conc. (ug/m <sup>3</sup> ) (2019)	Highest 24-Hour Conc. Site AQS ID	Number of SLAMS		
					Required <sup>a</sup>	Active	Additional Needed
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	54	Bethel Island 06-013-1002	2-4	2	0
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	130 <sup>b</sup>	Hollister 06-069-0002	4-8 <sup>b</sup>	2 <sup>c</sup>	2
Santa Rosa-Petaluma	Sonoma	483,878	85	Healdsburg 06-097-0002	0-1	3 <sup>d</sup>	0
Vallejo	Solano	413,344	70	Vacaville 06-095-3001	0-1	1 <sup>e</sup>	0
Napa	Napa	136,484	37	Napa Valley College 06-055-0004	0	0	0

<sup>a</sup> The number of PM<sub>10</sub> monitors required depends on the population of the MSA and the ambient concentration of PM<sub>10</sub> as described in Table D-4 of Appendix D, Part 58 of 40 CFR.

<sup>b</sup> Existing monitoring meets the needs of the local air districts and the communities, and the Air District will continue to assess the adequacy of the PM<sub>10</sub> networks in each 5-Year Network Assessment to determine if events like this become more common and drive the need for additional monitoring. The Air District is committed to working with EPA, CARB, and other local air districts to ensure that monitoring levels continue to protect public health and safety.

<sup>c</sup> One of the two monitors is not in the BAAQMD. It is in Hollister, which is in the Monterey Bay Unified APCD.

<sup>d</sup> These monitors are not in the BAAQMD. They are in Healdsburg, Guerneville, and Cloverdale, which are in the Northern Sonoma APCD.

<sup>e</sup> This monitor is not in the BAAQMD. It is in Vacaville, which is in the Yolo-Solano AQMD.

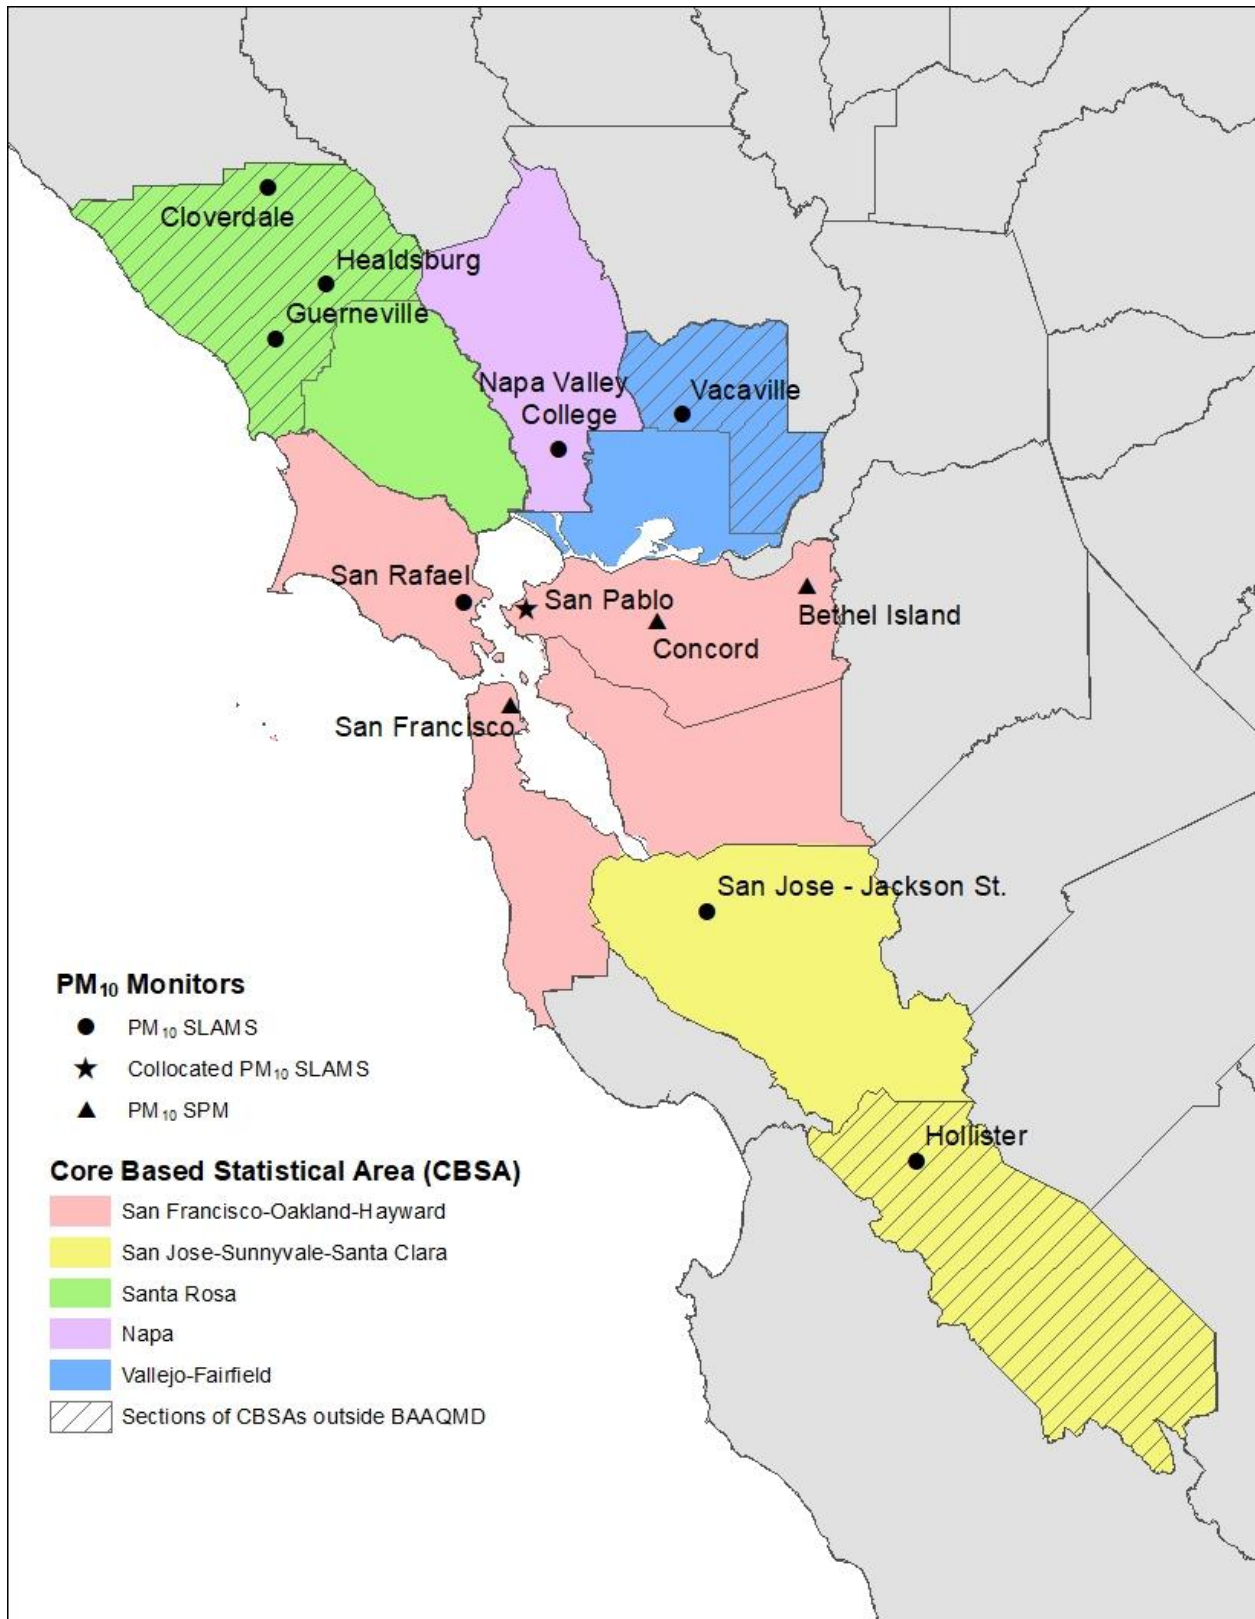


Figure 2-5. PM<sub>10</sub> Monitoring in the San Francisco Bay Area in 2019

## 2.2.4 Minimum Monitoring Requirements for Collocated PM<sub>10</sub>

EPA requires a PQA's network of manual PM<sub>10</sub> samplers to have collocated monitoring at 15% (or at least one) of the monitoring sites within a PQA (40 CFR 58, Appendix D §3.3.4). All primary PM<sub>10</sub> SLAMS in the Bay Area network are manual methods (method codes 063, 141, and 127). Table 2-9 summarizes the collocation of PM<sub>10</sub> in the Bay Area during 2018.

Table 2-9. Collocated PM<sub>10</sub> Monitoring in the Bay Area in 2019

Methods Codes	Number of Primary Manual SLAMS	Number of Required Collocated Manual SLAMS	Number of Active Collocated Manual SLAMS
063, 141, 127	4	1	1 San Pablo

Collocated PM<sub>10</sub> monitoring was moved to San Pablo on October 17, 2016 since the site could accommodate the logistics of collocation. It is an appropriate collocation site because the maximum concentrations at these sites are amongst the highest in the PQA and the concentrations are relatively consistent throughout the network.

Although the collocated sampler is only required to operate on a 1:12 schedule, the Bay Area operates the sampler 1:6 throughout the year; the collocated sampling frequency may be reevaluated in the future.

## 2.2.5 Minimum Monitoring Requirements for SO<sub>2</sub>

In 2019 the Air District operated eight SO<sub>2</sub> SLAMS and one SPM SO<sub>2</sub> monitor (Figure 2-6).

The number of required SO<sub>2</sub> monitors in each CBSA is determined by the product of the total amount of SO<sub>2</sub> emissions in the CBSA and its population as specified in 40 CFR 58, Appendix D §4.4.2 (Table 2-10). The resulting value is defined as the Population Weighted Emissions Index (PWEI). One SO<sub>2</sub> monitor is required in CBSAs with PWEI values greater than 5,000 but less than 100,000, and none when the value is less than 5,000. SO<sub>2</sub> emissions shown in Table 2-10 are from the 2014 National Emissions Inventory (NEI). Table 2-10 also shows that the Air District monitoring network meets or surpasses the SO<sub>2</sub> minimum requirements for monitoring by the PWEI.

In addition to minimum monitoring requirements by the PWEI, EPA requires trace-level SO<sub>2</sub> monitoring at NCore sites (40 CFR 58, Appendix D §4.4.5), which is fulfilled by a trace-level SO<sub>2</sub> monitor at the San Jose – Jackson NCore site.

The Data Requirements Rule (DRR) for the 2010 1-hour SO<sub>2</sub> NAAQS also requires monitoring or modeling to characterize ambient SO<sub>2</sub> concentrations near SO<sub>2</sub> sources that emit more than 2,000 tons per year (tpy). While there is no single source in the Bay Area that exceeds this emission threshold, EPA required further air quality characterization of the following sources in Martinez, a city in the San Francisco-Oakland-Hayward CBSA: the Shell Refinery, Tesoro Refinery, and Eco Services Sulfuric Acid Plant. In 2016, EPA approved the SO<sub>2</sub> SLAMS in Martinez as meeting this requirement.

The Air District may add additional SO<sub>2</sub> SLAMS around the five refineries to further characterize the air quality in the communities near refineries per our Regulation 3, and Regulation 12, Rule 15.

Finally, no additional SO<sub>2</sub> monitors are required for SIP or Maintenance Plans because the Air District has never been designated as nonattainment for SO<sub>2</sub> and, therefore, no SIP or maintenance plans have been prepared for SO<sub>2</sub>. EPA has designated the entire state of California as Attainment/Unclassifiable as of December 2017.

### **SO<sub>2</sub> Special Purpose Monitor**

The Crockett SO<sub>2</sub> monitor is too close to a nearby tree to meet 40 CFR 58 Appendix E siting requirements. Therefore, it is designated a source-oriented SPM and is not counted towards minimum monitoring requirements. However, this monitor meets the requirements of 40 CFR 58 Appendix A and is, therefore, considered to be comparable to the NAAQS, in that, a violation of the NAAQS measured at the site is still valid.

Table 2-10. Minimum Monitoring Requirements for SO<sub>2</sub>

MSA	County or Counties	Population <sup>a</sup> 2010 Census	Total SO <sub>2</sub> (tons/yr) 2017 NEI	PWEI (million- person- tons/yr)	Number of SLAMS		
					Required	Active	Additional Needed
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	3350	14522	1 <sup>a</sup> (PWEI and DRR)	6	0
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	1637	3008	1 <sup>b</sup> (NCore)	1	0
Santa Rosa-Petaluma	Sonoma	483,878	1	0.5	0	0	0
Vallejo	Solano	413,344	76	31	0	1	0
Napa	Napa	136,484	0	0	0	0	0

<sup>a</sup> There is a requirement for one SO<sub>2</sub> monitor both from the PWEI and from the final SO<sub>2</sub> DRR. These requirements could be met by the same monitor, so the requirement is listed as one monitor. However, the Air District intends to continue operating more SO<sub>2</sub> monitors than are required to characterize the effects of sources in this CBSA.

<sup>b</sup> A trace-level SO<sub>2</sub> monitor is required at the San Jose – Jackson site (06-085-0005) for NCore (40 CFR 58, Appendix D §4.4.5). There are no monitoring requirements by PWEI for the San Jose-Sunnyvale-Santa Clara CBSA.



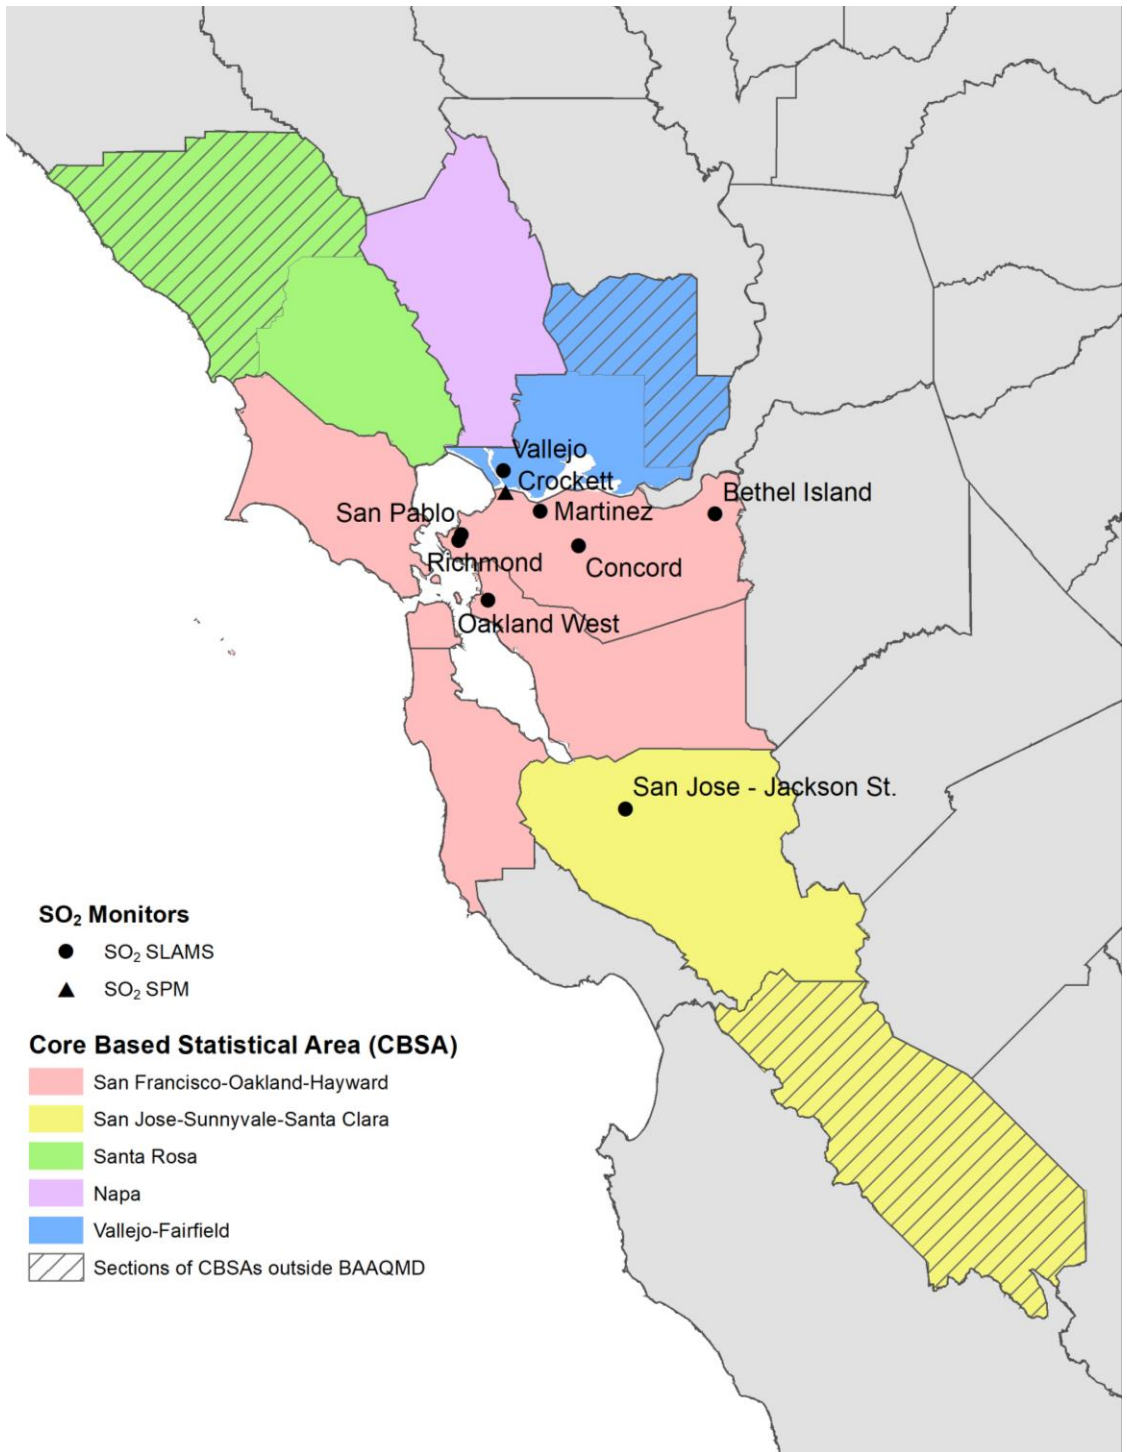


Figure 2-6. SO<sub>2</sub> Monitoring in the San Francisco Bay Area in 2019

## 2.2.6 Minimum Monitoring Requirements for NO<sub>2</sub>

On April 12, 2010, EPA revised the minimum monitoring requirements for NO<sub>2</sub> in 40 CFR Part 58, Appendix D §4.3. The revision required the Air District to operate NO<sub>2</sub> monitors at neighborhood-scale or larger sites to monitor the expected highest area-wide concentrations, and at sites within 50 meters of major freeways (near-road sites). In addition, the rule required the EPA Regional Administrators to identify an additional 40 sites nationwide to monitor NO<sub>2</sub> in areas with susceptible and vulnerable populations by January 1, 2013. In implementing this requirement, EPA selected existing area-wide SLAMS in important areas with susceptible and vulnerable populations, if one existed, to meet this requirement.

On March 7, 2013 and December 30, 2016, EPA issued final rules revising the requirements and implementation dates for near-road NO<sub>2</sub> sites. The current requirements are for one near-road NO<sub>2</sub> monitor in CBSA's with a population greater than 1 million, and a second near-road NO<sub>2</sub> monitor in CBSA's with a population greater than 2.5 million or CBSA's with populations over 1 million and roadway with annual average daily traffic (AADT) over 250,000. Based on CBSA population and traffic counts, the Air District was initially required to operate three near-road monitoring sites. In addition to the near-road monitoring requirement, the Air District is required to monitor for area-wide NO<sub>2</sub> concentrations at one site in both the San Francisco-Oakland-Berkeley and the San Jose-Sunnyvale-Santa Clara CBSAs (see Table 2-12).

No additional monitors are required for the SIP or Maintenance Plans because the Air District is not designated as non-attainment for NO<sub>2</sub> and no SIP or maintenance plans have been prepared for NO<sub>2</sub>.

As part of the NO<sub>2</sub> network design criteria, EPA sets the most important scale for different NO<sub>2</sub> monitoring objectives. The most important spatial scale for near-road NO<sub>2</sub> monitoring stations to effectively characterize the maximum expected hourly NO<sub>2</sub> concentration due to mobile source emissions on major roadways is microscale. The most important spatial scales for other monitoring stations characterizing maximum expected hourly NO<sub>2</sub> concentrations are microscale and middle scale. The most important spatial scale for area-wide monitoring of high NO<sub>2</sub> concentrations is neighborhood scale.

In 2019, the Air District operated ten area-wide neighborhood scale NO<sub>2</sub> SLAMS in the Bay Area, including six in the San Francisco-Oakland-Berkeley CBSA and one in the San Jose-Sunnyvale-Santa Clara CBSA. One of the ten, the Oakland West site, was selected as one of the 40 nationwide sites for monitoring NO<sub>2</sub> in areas with susceptible and vulnerable populations.

Table 2-11 shows the various spatial scales of the NO<sub>2</sub> SLAMS and SPMs in each CBSA. NO<sub>2</sub> monitoring at Oakland East, San Rafael, and San Pablo is middle scale based on traffic counts and the distance between the monitors and the nearest traffic lane to the monitors. Therefore, these sites, like the near-road sites, are not counted toward meeting the area-wide requirements of 40 CFR Part 58, Appendix D §4.3.3.

Table 2-12 shows NO<sub>2</sub> minimum monitoring requirements by CBSA for near-road and area-wide monitoring; Figure 2-7 is a map of the NO<sub>2</sub> SLAMS and SPMs in the Bay Area.

In 2019, the Air District continued to meet the NO<sub>2</sub> minimum monitoring requirements for area-wide and Regional Administrator Required Monitoring in areas with susceptible and vulnerable populations. The Air District also meets the near-road NO<sub>2</sub> minimum monitoring requirements in the San Francisco-Oakland-Berkeley CBSA with the addition of the Berkeley Aquatic Park (near-road) station in 2019. While there have been decreases in the traffic counts in the San Jose-Sunnyvale-Santa Clara CBSA since 2017, one road segment in the ABSA still exceeds the 250,000 AADT threshold for a second near-road NO<sub>2</sub> site in a CBSA. After consulting with EPA, the appropriate timeframe for addressing this requirement is in the network assessment to be submitted to EPA in 2020. The Air District will consider whether traffic amounts are expected to remain consistently above the threshold, the variation in the existing four near road sites in the Bay Area, and whether EPA has determined whether there are resources to fund additions to the near-road NO<sub>2</sub> network.

### **NO<sub>2</sub> Special Purpose Monitor**

San Ramon is a NO<sub>2</sub> SPM, operated as part of the Air District's voluntary PAMS program, and meets the requirements of 40 CFR Part 58, Appendices E and A. In 2019, San Ramon was operated year-round. Therefore, NO<sub>2</sub> data meets the data completeness requirement and can be compared to the NAAQS but cannot be counted towards meeting the minimum monitoring requirements.

Table 2-11. NO<sub>2</sub> Monitors at Various Spatial Scales

<b>CBSA</b>	<b>County or Counties</b>	<b>Population 2010 Census</b>	<b>Sites at Micro Scale<sup>a</sup></b>	<b>Sites at Middle Scale<sup>a</sup></b>	<b>Sites at Neighborhood Scale or Greater</b>
San Francisco-Oakland-Berkeley	San Francisco, San Mateo, Alameda, Marin, Contra Costa	4,335,391	Laney College, Berkeley Aquatic Park, Pleasanton <sup>b</sup>	Oakland East, San Pablo, San Rafael	Bethel Island, Concord, Livermore, Oakland West, Redwood City, San Francisco, San Ramon <sup>b</sup>
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	San Jose-Knox	None	San Jose-Jackson
Santa Rosa-Petaluma	Sonoma	483,878	None	None	Sebastopol
Vallejo	Solano	413,344	None	None	Vallejo
Napa	Napa	136,484	None	None	Napa Valley College

<sup>a</sup> Micro- and middle-scale sites are not counted towards meeting the requirement for monitoring area-wide concentrations.

<sup>b</sup> Pleasanton and San Ramon are SPMs and are not counted toward meeting the requirement for monitoring near-road and area-wide concentrations, respectively.

Table 2-12. Minimum Monitoring Requirements for NO<sub>2</sub>

CBSA	Population 2010 Census	Maximum AADT (2018 <sup>a</sup> )	Road Segment for Max AADT	Near-road Monitors			Area-wide Monitors		
				Required	Active	Additional Needed	Required	Active	Additional Needed
San Francisco-Oakland-Berkeley	4,335,391	291,000	Walnut Creek, North Main St., Rte. 680	2	3	0	1 <sup>b</sup>	6	0
San Jose-Sunnyvale-Santa Clara	1,836,911	275,800	San Jose, Tully Road, Rte. 101	2 <sup>c</sup>	1 <sup>d</sup>	1 <sup>c</sup>	1	1	0
Santa Rosa-Petaluma	483,878	157,300	Baker Avenue, Rte. 101	0	0	0	0	1	0
Vallejo	413,344	232,000	Suisun Valley Road, Rte. 80	0	0	0	0	1	0
Napa	136,484	134,000	Solano/Napa County Line, Rte. 80	0	0	0	0	1 <sup>e</sup>	0

<sup>a</sup> Traffic volume data was taken from CalTrans estimates here: [https://gisdata-caltrans.opendata.arcgis.com/datasets/f71f49fb87b3426e9688fe66039170bc\\_0](https://gisdata-caltrans.opendata.arcgis.com/datasets/f71f49fb87b3426e9688fe66039170bc_0)

<sup>b</sup> One area-wide monitor is required; additionally, the Oakland West monitoring site was selected by EPA as one of the 40 nationwide sites for monitoring near susceptible and vulnerable populations. Since the two requirements for this CSBA can be met by the same site, there is only one required monitor in this CBSA.

<sup>c</sup> Recent increases in traffic triggered a second required monitor in the San Jose-Sunnyvale-Santa Clara CBSA. The plan for implementing this site will be included in the next Five-Year Network Assessment due to EPA by July 1, 2020.

<sup>d</sup> This monitor is shared with Monterey Bay Unified APCD. The monitoring agreement is in Appendix C.

<sup>e</sup> NO<sub>2</sub> at Napa is monitored at middle scale based on distance to the roadway and traffic count which cannot be counted as an area-wide monitor. The NO<sub>2</sub> sensor at Napa Valley College (replacement for Napa site) is monitored at neighborhood scale. Therefore, it can be counted as an area-wide monitor.

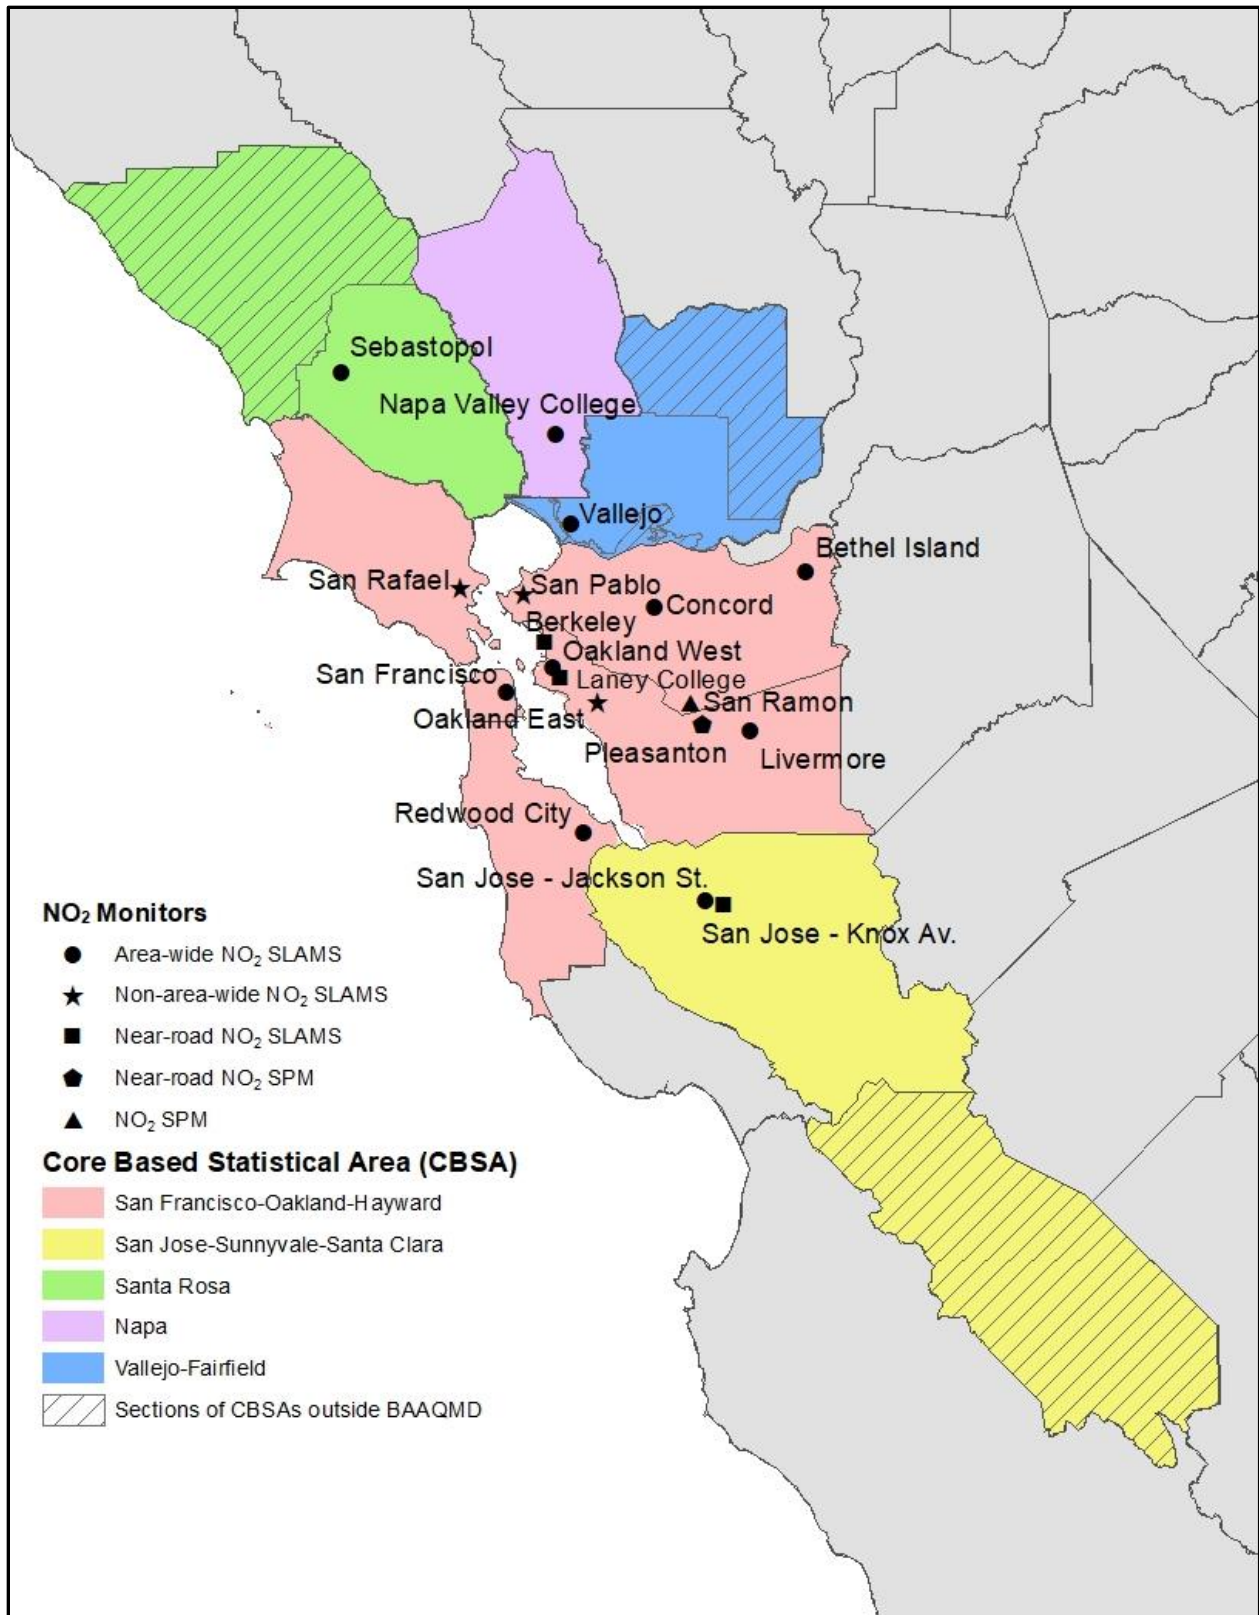


Figure 2-7. NO<sub>2</sub> Monitoring in the San Francisco Bay Area in 2019s

## 2.2.7 Minimum Monitoring Requirements for CO

Effective October 31, 2011, EPA revised 40 CFR Part 58, Appendix D for carbon monoxide (CO) monitoring. The revision requires one CO monitor to operate collocated with a near-road NO<sub>2</sub> monitor in CBSAs having a population of 1 million or more. If a CBSA is required to have more than one near-road NO<sub>2</sub> monitor, only one CO monitor is required to be collocated with a near-road NO<sub>2</sub> monitor within that CBSA. Table 2-13 shows these requirements applied to the Bay Area CBSAs. The Air District operates CO monitors at all near-road sites, and meets the minimum monitoring requirements for CO.

Table 2-13. Minimum Monitoring Requirements for CO

<b>CBSA</b>	<b>County or Counties</b>	<b>Pop. 2010 Census</b>	<b>Near-road Monitors Required</b>	<b>Near-road Monitors Active</b>	<b>Near-road Monitors Needed</b>
San Francisco-Oakland-Berkeley	SF, San Mateo, Alameda, Marin, Contra Costa	4,335,391	1	2	0
San Jose-Sunnyvale-Santa Clara	Santa Clara, San Benito	1,836,911	1	1 <sup>a</sup>	0
Santa Rosa-Petaluma	Sonoma	483,878	0	0	0
Vallejo	Solano	413,344	0	0	0
Napa	Napa	136,484	0	0	0

<sup>a</sup> This monitor will be shared with Monterey Bay Unified APCD. The monitoring agreement is in Appendix D.

In addition to minimum monitoring requirements for near-road CO, EPA requires trace-level CO monitoring at NCore sites (40 CFR 58, Appendix D §4.4.5), which is fulfilled by a trace-level CO monitor at the San Jose-Jackson NCore site (06-085-0005).

The Air District was redesignated attainment for the CO 8-hour NAAQS in 1998. The Air District CO maintenance plan is contained within the California Air Resource Board document "2004 Revision to the California State Implementation Plan for Carbon Monoxide." The plan does not specify the number of CO monitors needed. In 2019, the Air District operated 17 CO monitors: one within each of the nine Bay Area counties plus additional CO monitors in large cities and four near-road CO monitors (Figure 2-8).



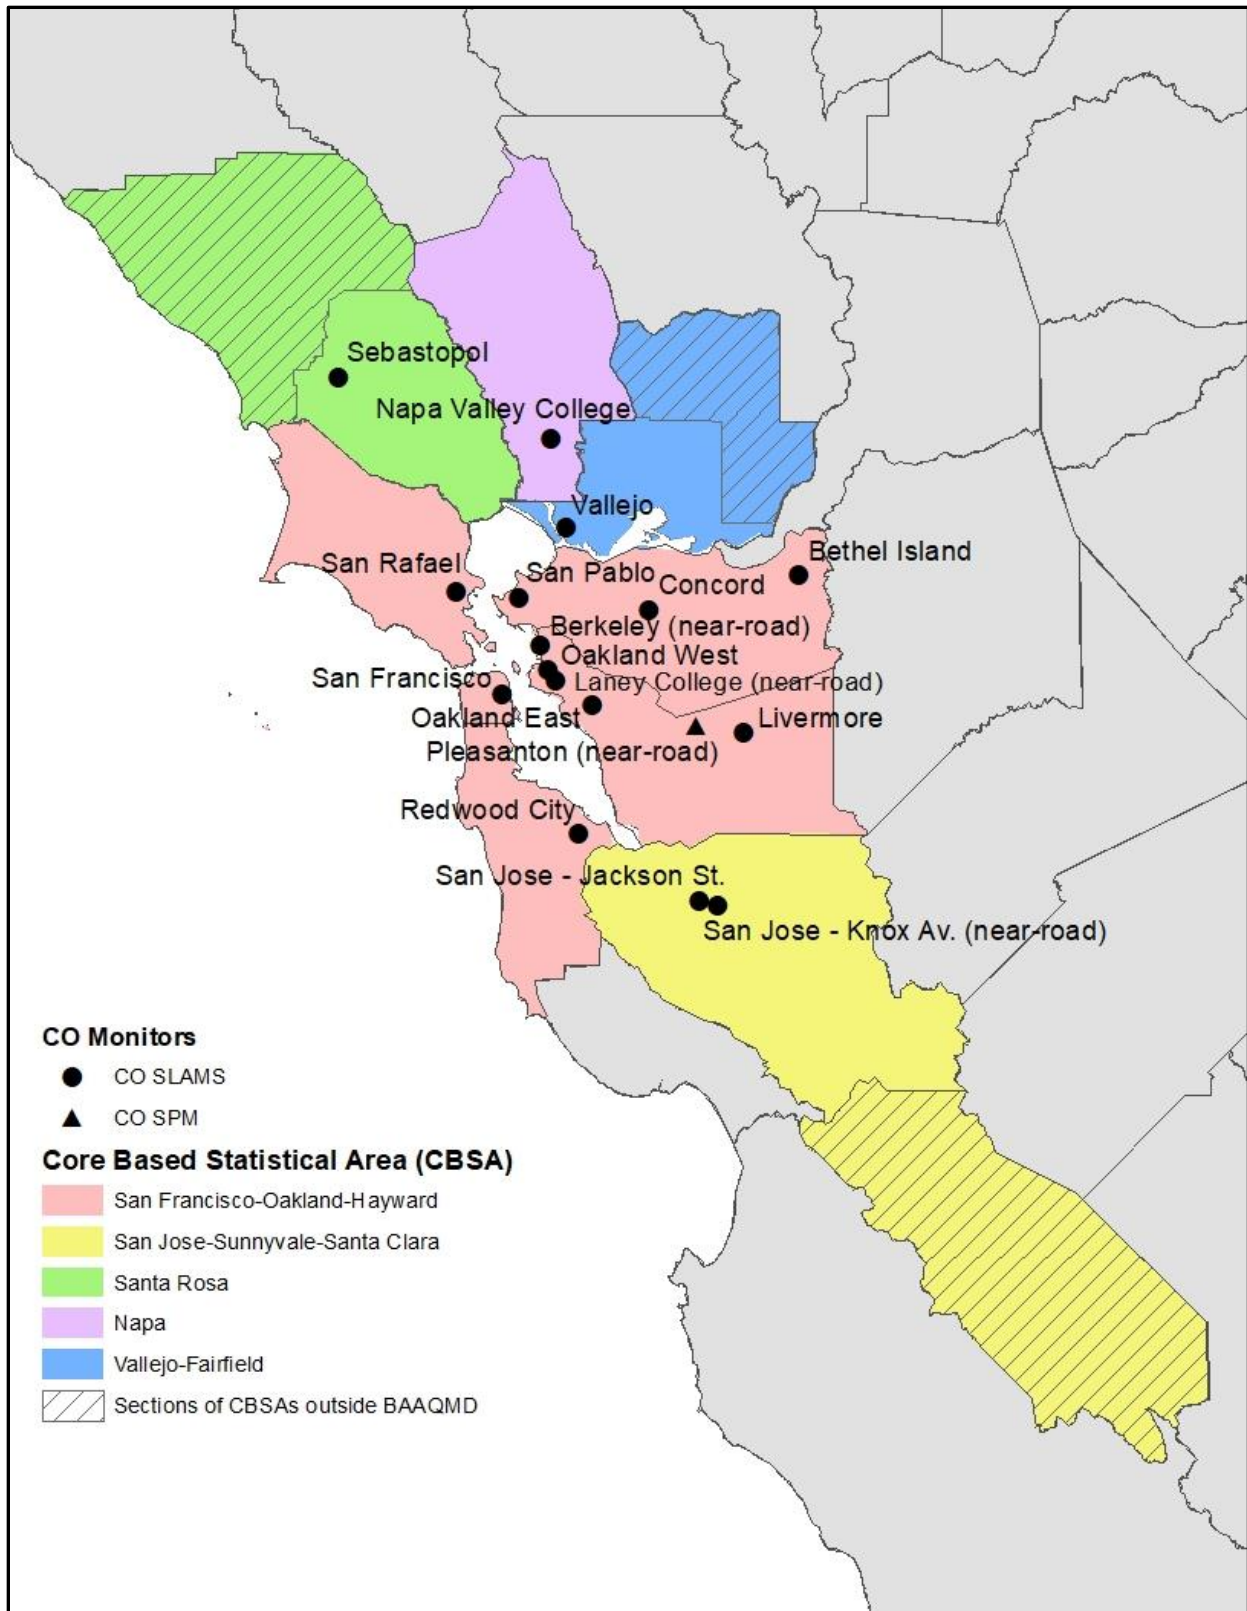


Figure 2-8. CO Monitoring in the San Francisco Bay Area in 2019



## 2.2.8 Minimum Monitoring Requirements for Lead

40 CFR Part 58, Appendix D §4.5(a) requires lead monitoring near sources expected to contribute to a maximum lead (Pb) concentration in ambient air in excess of the NAAQS. These monitors are to be sited, considering logistics and the potential for population oriented, where the ambient Pb concentration is expected to be at its maximum. The applicable sources are identified by having emissions greater than 0.5 tpy for non-airport sources and greater than 1.0 tpy for airports. In the Bay Area there are no sources meeting this criterion according to the 2014 National Emissions Inventory (NEI). However, 40 CFR Part 58, Appendix D §4.5(a)(iii) requires source-oriented monitoring near an additional 15 airports to evaluate air quality near airports with emissions from piston engine aircraft using leaded fuel that may approach 0.50 tons per year, including three airports in the Bay Area (Palo Alto, San Carlos, and Reid-Hillview). One of the airport lead monitoring sites is also required to operate a collocated sampler.

The Palo Alto Airport lead site was shut down at the end of December 2014 because Santa Clara County sold the property to the city of Palo Alto. The sale triggered FAA review of various operational plans and permits, revealing that the lead sampler location violated FAA regulations. The Air District continues to work with EPA to find a suitable alternative.

The San Carlos Airport lead monitoring site was moved about 120 yards to the southeast because the property owner at the original site did not renew the lease. Data collected at the original site ended on September 13, 2013 and resumed at the new location (San Carlos II) on March 25, 2015.

As of Tuesday, April 11, 2017, the TSP-Pb monitoring at the San Carlos Airport II monitoring site has been discontinued due to circumstances beyond the Air District's control. The San Carlos Airport management informed the Air District site operator on April 11 that the Air District is no longer allowed access to the site, citing the expired lease. The Air District has tried unsuccessfully to renegotiate the lease since November 2016. The airport management is requiring that a shutdown provision be included in the renewed lease. However, the Air District cannot commit to the provision, since EPA, not the Air District, has the authority to approve the closure of the site. The Air District notified EPA of the discontinuation of data collection on April 13, 2017. The Air District continues to work with EPA to find a suitable alternative.

Figure 2-9 shows the lead monitors in the San Francisco Bay Area in 2019. Minimum monitoring requirements for source-oriented lead at airports and NATTS site at San Jose are provided in Tables 2-14 and 2-15.

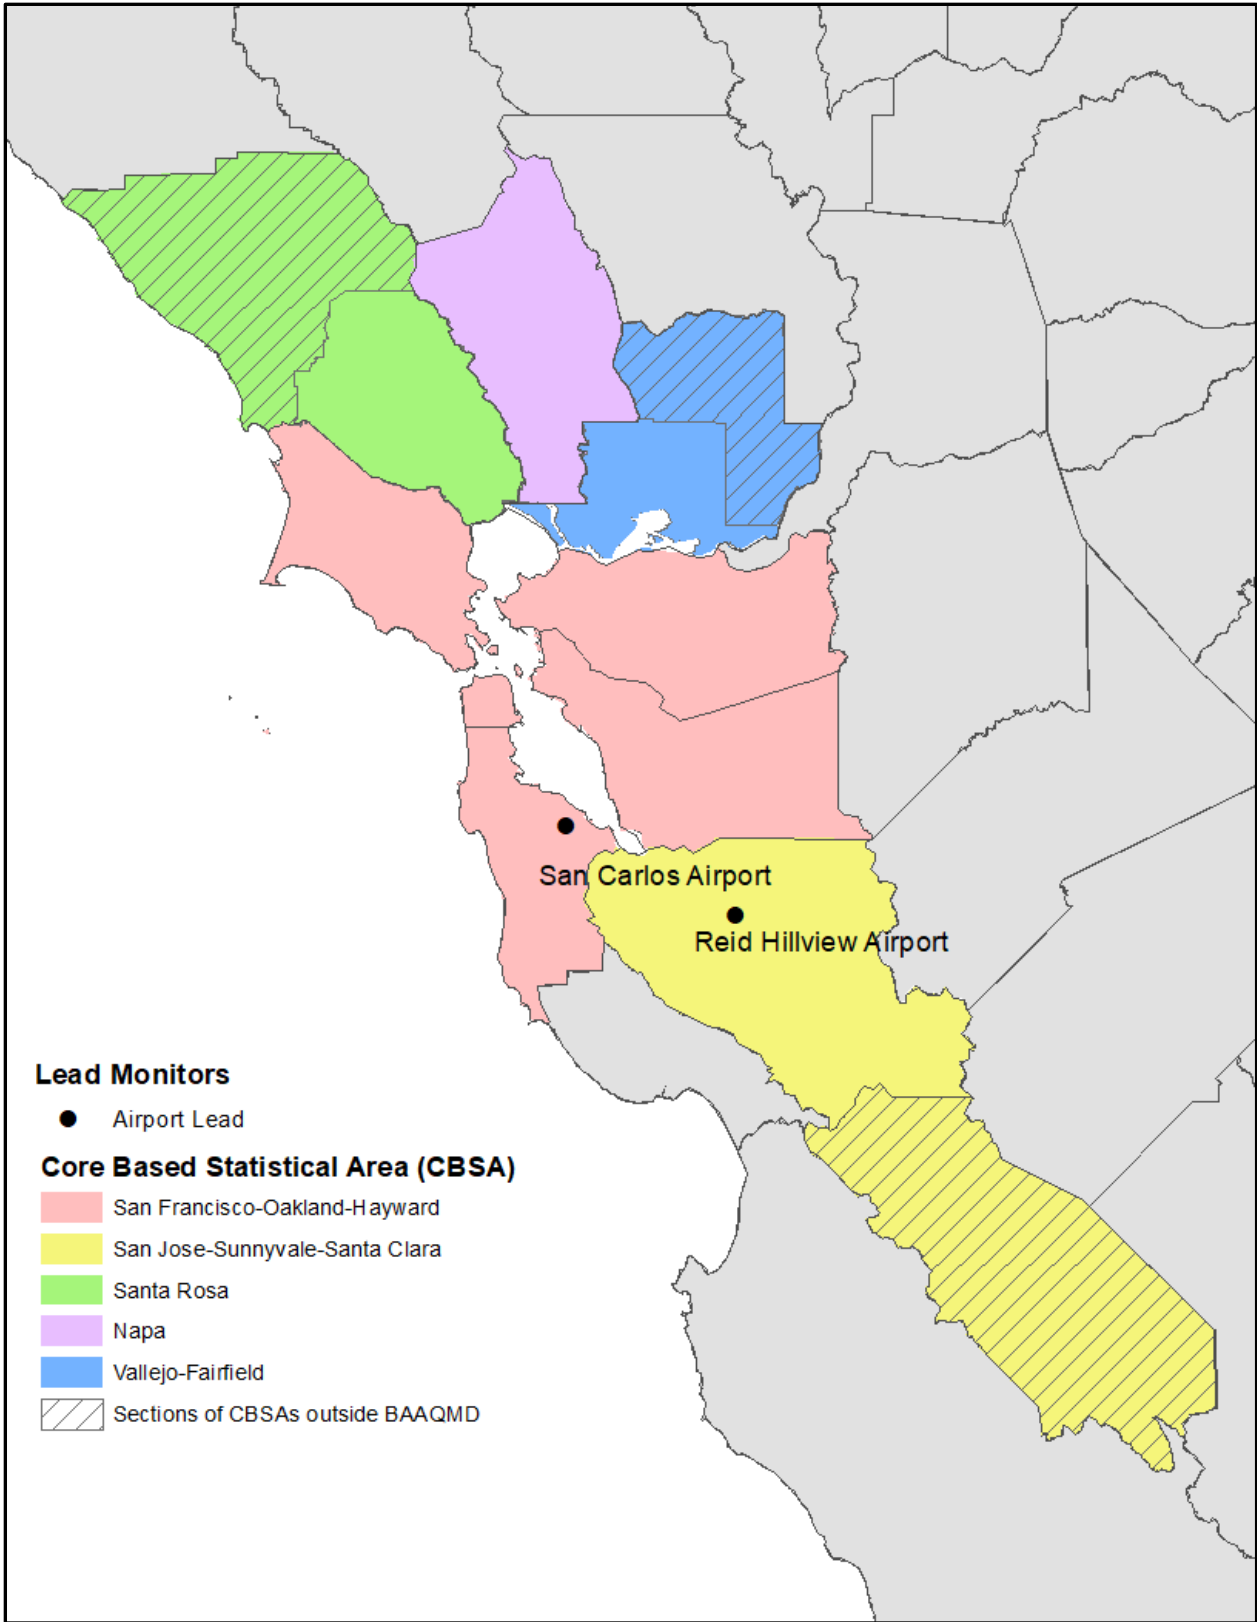


Figure 2-9. Lead Monitoring in the San Francisco Bay Area in 2019

Table 2-14. Source Oriented Lead Monitoring at Airports

Source Name	Address	Lead Emissions (tons/yr) 2017 NEI	Number of SLAMS		
			Required	Active	Additional Needed
San Carlos Airport	620 Airport Way San Carlos 94070	0.30	1	0 <sup>a</sup>	1 <sup>a</sup>
Palo Alto Airport	1925 Embarcadero Rd. Palo Alto 94303	0.48	1	0 <sup>b</sup>	1 <sup>b</sup>
Reid-Hillview Airport	2500 Cunningham Ave. San Jose 95148	0.37	1	1	0

<sup>a</sup> The San Carlos Airport II monitor began operation on March 25, 2015. On Tuesday, April 11, 2017, the San Carlos Airport II monitor was shut down due to an expired lease and the inability to come to terms with a new lease.

<sup>b</sup> The Palo Alto monitor was shut down in December 2014, after it was found to violate FAA regulations and would therefore need to be relocated. EPA and the Air District are working to identify a suitable location so that lead monitoring can resume at this airport.

Table 2-15. Collocated Source Oriented Lead Monitoring at Airports

Source Name	Address	Lead Emissions (tons/yr) 2014 NEI	Collocated Monitors Required	Active Monitors	Additional Monitors Needed
San Carlos Airport	620 Airport Way San Carlos 94070	0.30	1	0 <sup>a</sup>	1 <sup>a</sup>

<sup>a</sup> The San Carlos Airport II sampler began operation on March 25, 2015. On Tuesday, April 11, 2017, the San Carlos Airport II monitor was shut down due to an expired lease and the inability to come to terms with a new lease.

## 2.3 Modifications Made to Network in 2019

There were no network modifications completed in 2019.

## 2.4 Proposed Modifications to Network in 2020–2021

### Community Monitoring Near Refineries

As a part of the Regulation 12, Rule 15 rulemaking process, the Air District has committed to conducting additional monitoring in communities near refineries, funded by fees paid by the facilities, per Regulation 3.

In 2018, the Air District conducted workshops to ask for public input on the cumulative impacts experienced in these areas. The Air District is evaluating the information submitted by the public, along with the most up-to-date source location, emissions, modeling, and ambient monitoring data to determine the best monitoring locations to further evaluate the exposure the nearby communities are experiencing, and will be looking for places that logistically accommodate a new fixed site at these locations throughout 2020.

### Hayward – Ozone Monitor

As noted in section 2.2.1, EPA noted in their 2018 TSA that the Hayward O<sub>3</sub> monitor does not meet 40 CFR 58 Appendix E siting requirements and that it should, therefore, be classified as an SPM. The Air District is requesting that EPA approve the closure of the Hayward ozone monitor as a SLAMS since it meets the criteria of 40 CFR 58.14 (c) and 58.14 (c) (2) which state:

*(c) State, or where appropriate, local agency requests for SLAMS monitor station discontinuation, subject to the review of the Regional Administrator, will be approved if any of the following criteria are met and if the requirements of appendix D to this part, if any, continue to be met. Other requests for discontinuation may also be approved on a case-by-case basis if discontinuance does not compromise data collection needed for implementation of a NAAQS and if the requirements of appendix D to this part, if any, continue to be met.*

...

*(2) Any SLAMS monitor for CO, PM<sub>10</sub>, SO<sub>2</sub>, or NO<sub>2</sub> which has consistently measured lower concentrations than another monitor for the same pollutant in the same county (or portion of a county within a distinct attainment area, nonattainment area, or maintenance area, as applicable) during the previous five years, and which is not specifically required by an attainment plan or maintenance plan, if control*

*measures scheduled to be implemented or discontinued during the next five years would apply to the areas around both monitors and have similar effects on measured concentrations, such that the retained monitor would remain the higher reading of the two monitors being compared.*

Figure 2-16 below shows that the Hayward site has never been the maximum concentration site for the San Francisco-Oakland-Berkeley CBSA nor for the San Francisco Bay Area nonattainment area. More specifically, the Livermore and San Martin sites, located in the Bay Area’s two maximum ozone areas downwind of urban precursors, have always measured higher design values than the Hayward site. Therefore, the discontinuation of the Hayward O<sub>3</sub> monitor as a SLAMS does not compromise data collection needed for implementation of the NAAQS. The Air District intends to continue operating the Hayward ozone monitor as an SPM as resources allow. If the SLAMS closure is approved, the Hayward O<sub>3</sub> SPM will not be counted towards minimum monitoring requirements in future years, however, the San Francisco-Oakland-Berkeley CBSA will still meet minimum monitoring requirements.

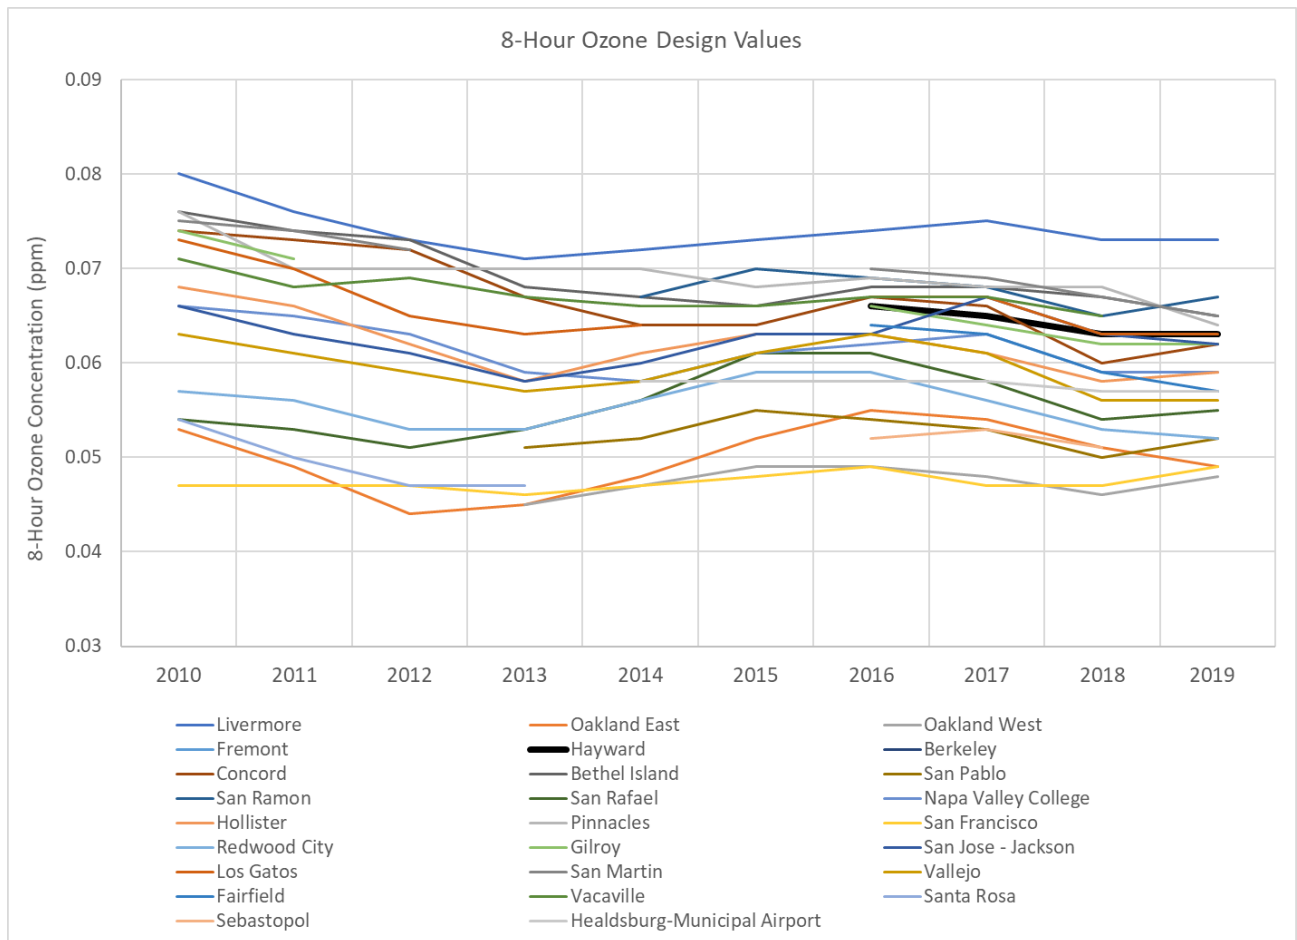


Figure 2-10. Ozone Design Values from 2010-2019

### Lead – Palo Alto Airport

In 2019, the Air District plans to request closure of the Palo Alto Airport lead site.

### Lead – San Carlos Airport II

As of Tuesday, April 11, 2017, the TSP-Pb monitoring at the San Carlos Airport II monitoring site has been discontinued due to circumstances beyond our control. The San Carlos Airport management informed the Air District site operator on April 11 that the Air District is no longer allowed access to the site, citing the expired lease. The Air District has tried unsuccessfully to renegotiate the lease since November 2016. The airport management is requiring that a shutdown provision be included in the renewed lease. However, the Air District cannot commit to the provision, since EPA, not the Air District, has the authority to approve the closure of the site. The Air District notified EPA of the discontinuation of data collection on April 13, 2017. In 2019, the Air District plans to request closure of the San Carlos Airport II site.

### Livermore - PAMS

The Air District is required to operate a core PAMS site beginning June 2021. EPA approved a waiver for the Air District to fulfill this requirement at the Livermore site rather than the San Jose – Jackson site since the Livermore site is critical for the Bay Area regional ozone modeling. See section 5.4 for additional details.

### Near-road Monitoring Update

In 2018, the Air District installed a near-road air monitoring site in Pleasanton near the intersections of Highways 580 and 680. This site was located at the request of an Air District Board member, and began operating in April 2018.

While there have been decreases in the traffic counts in the San Jose-Sunnyvale-Santa Clara CBSA since 2017, one road segment in the ABSA still exceeds the 250,000 AADT threshold for a second near-road NO<sub>2</sub> site in a CBSA. After consulting with EPA, the appropriate timeframe for addressing this requirement is in the network assessment to be submitted to EPA in 2020. The Air District will consider whether traffic amounts are expected to remain consistently above the threshold, the variation in the existing four near road sites in the Bay Area, and whether EPA has determined whether there are resources to fund additions to the near-road NO<sub>2</sub> network.

### San Jose NO<sub>y</sub> monitoring for NCore

In October 2017, the Air District received approval from EPA to discontinue NO<sub>y</sub> monitoring because the past three years of data showed an insignificant statistical difference between NO<sub>x</sub> and NO<sub>y</sub>. The waiver approval is in Appendix G. EPA approved this request and the Air District intends to operate the NO<sub>y</sub> monitor year-round at the Livermore site (rather than at San Jose – Jackson) when the newly required PAMS monitoring commences.

## 2.5 Removing a NAAQS Compliance Monitor

When the Air District proposes changes to the air monitoring network, the proposed changes are included in the Annual Monitoring Network Plan. The Annual Monitoring Network Plan is posted on the Air District website for 30 days for public comment on the proposed changes. After the public comment period, the Air District reviews and considers the comments before making a final decision on a change to air monitoring network. The Air District submits the Annual Monitoring Network Plan with public comments to the EPA Region 9 Regional Administrator by July 1 each year.

Before shutting down a SLAMS (State or Local Air Monitoring Station) monitor, 40 CFR Part 58.14(c) requires that the Air District obtain the Regional Administrator's written approval. The Regional Administrator will normally approve the shutdown of a SLAMS monitor when any of the following situations apply:

1. Criteria pollutant monitors which have shown attainment of the national standards during the previous five years may be removed if the probability is less than 10% that the monitor will exceed 80% of NAAQS during the next three years, and if the monitor is not required by an attainment or maintenance plan.
2. CO, PM<sub>10</sub>, SO<sub>2</sub>, or NO<sub>2</sub> monitors not required by an attainment or maintenance plan may be removed if the monitor has shown consistently lower concentrations than another monitor for the same pollutant in the same county during the previous five years and is expected to remain higher during the following five years given expected implementation of control measures in the area.
3. Criteria pollutant monitors that have not violated the national standards in the most recent five years may be removed if the State Implementation Plan (SIP) provides a method of representing the air quality in the applicable county in the absence of monitoring.
4. PM<sub>2.5</sub> monitors may be removed when EPA determines that measurements are not comparable to the relevant NAAQS because of siting issues in accordance with 40 CFR 58.30.
5. Criteria pollutant monitors that are located upwind of an urban area to characterize transport into the area may be removed if the monitor has not recorded violations of the relevant NAAQS in the previous five years and the monitor is being replaced by another monitor characterizing transport.
6. Criteria pollutant monitors not eligible for removal under any of the above criteria may be relocated to a nearby location with the same scale of representation if logistical problems beyond the agency's control make it impossible to continue operation at its current site.



EPA may also approve other requests for discontinuation on a case-by-case basis if discontinuance does not compromise data collection needed for implementation of a NAAQS and if the requirements of 40 CFR Part 58, Appendix D continue to be met.

The closure of an SPM (Special Purpose Monitor) monitor does not require approval from EPA (see 40 CFR 58.20(f)), but changing in the monitor type from SLAMS to SPM requires approval of the Regional Administrator.

## **2.6 Data Submission Requirement**

After all data review procedures are complete, the Air District submits monthly air quality and associated precision and accuracy reports to the EPA AQS database within 90 days of the end of every month. By May 1 each year, the Air District submits a data certification letter to Region 9 stating that the previous calendar year of data is complete and correct. The certification letter for 2018 data was submitted to EPA Region 9 on May 1, 2019.

### 3. SITE INFORMATION DEFINITIONS

Section 4 describes each of the 35 air quality sites operating within the Bay Area Air Quality Management District in 2018. The site descriptions include siting information about the site and a general description of the individual monitors at the site and their purpose. Monitors that are operated to determine compliance with the NAAQS must be operated following EPA requirements found in 40 CFR Part 58. These regulations also specify monitor siting criteria for each pollutant.

Included in each site description is also the number of days when a criteria pollutant measurement exceeded the National Ambient Air Quality Standard (NAAQS). The national standards for hourly and daily averaging times are shown in Table 3-1 below. The table below is abbreviated for clarity. A full list of national and California ambient air quality standards and the Air District's attainment status for each pollutant can be viewed at: <http://www.baaqmd.gov/research-and-data/air-quality-standards-and-attainment-status>.

Table 3-1. National Ambient Air Quality Standards (as of December 31, 2015)

Pollutant	Averaging Time	Standard
Ozone	8 hour	0.070 ppm
PM <sub>2.5</sub>	24 hour	35 µg/m <sup>3</sup>
PM <sub>2.5</sub>	1 year	12.0 µg/m <sup>3</sup>
PM <sub>10</sub>	24 hour	150 µg/m <sup>3</sup>
Carbon Monoxide	1 hour	35 ppm
	8 hour	9 ppm
Sulfur Dioxide	1 hour	75 ppb
Nitrogen Dioxide	1 hour	100 ppb
Lead	Rolling 3-month average	0.15 µg/m <sup>3</sup>

More detailed information about NAAQS standards, including past standards, may be found at: <https://www.epa.gov/criteria-air-pollutants/naaqs-table>. Table 3-2 explains the monitoring terms and definitions used in the detailed site summaries found in the site information sections later in this document.

Table 3-2. Monitor Information Definitions and EPA Air Monitoring Siting Criteria

Site or Monitor Information	Definition of Terms
AQS ID	The 9-digit code that identifies each site in the EPA's AQS database
GPS coordinates (decimal degrees)	The latitude and longitude of the site from the World Geodetic System (WGS-84) used as the reference coordinate system for Global Positioning System (GPS).
Distance to roadways from the gaseous probe (meters)	40 CFR Part 58 Appendix E, 6.0: specifies the distance monitors must be from roadways to be considered neighborhood- or urban-scale. Recommended distances are found in Table E-1 for NO <sub>x</sub> and O <sub>3</sub> , Table E-2 for CO, and Figure E-1 for PM.
Traffic count	The annual average daily traffic (AADT) count.
Groundcover	40 CFR Part 58 Appendix E, 3.0: states that particulate samplers should not be located in an unpaved area unless there is vegetative ground cover year round, so that the impact of wind-blown dusts will be kept to a minimum.
Statistical Area	The core based statistical area (CBSA) or Metropolitan Statistical Area (MSA) the site is located within.
Pollutant, POC	The pollutant being measured and its Parameter Occurrence Code (POC). There may be multiple instruments measuring a pollutant at a site. Each instrument of the same pollutant is assigned a unique POC to differentiate it from the others in EPA's AQS database.
Primary/QA Collocated/Other	This row applies to parameters that have collocation requirements as well as parameters that are combined at a site level for design value calculations. This currently includes PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10-2.5</sub> , Pb and NO <sub>2</sub> . Non-PM, Pb, and NO <sub>2</sub> monitors are listed as "N/A".
Parameter code	The 5-digit code assigned to each pollutant in the EPA's AQS database.
Basic monitoring objective(s)	The purpose for monitoring at that location. Choices include public information, NAAQS comparison, and research.
Site type(s)	Choices include highest concentration, population oriented, source impact, general/background, regional transport, and welfare-related impacts.
Monitor type(s)	Choices include SLAMS, Special Purpose (SPM), Industrial, Non-EPA Federal, Tribal, EPA and Other.
Network affiliation(s)	Some monitors are used for specific types of monitoring networks. Examples that apply to the Bay Area include: CSN STN, CSN Supplemental, NATTS, NCore, Near Road, and Unofficial PAMS. The full list may be found at: <a href="https://aqsweb/documents/codetables/networks.html">https://aqsweb/documents/codetables/networks.html</a>
Instrument manufacturer and model	Details about the instrumentation used to measure the pollutant.

Site or Monitor Information	Definition of Terms
Method code	Based on the Instrument manufacture and model, a method code is assigned and is reported to the EPA AQS database system. 40 CFR Part 58 Appendix C, 2.0: requires that the monitor used must be from EPA's current List of Designated Reference and Equivalent Methods.
FRM/FEM/ARM/other	FRMs (Federal Reference Methods) and FEMs (Federal Equivalent Methods) are approved by EPA for criteria pollutant monitoring to determine compliance with the. An ARM (Approved Regional Method) may be approved by EPA as an alternative to and FRM or FEM, however, no ARMs are used in the Bay Area.
Collecting Agency	The agency that operates the instrument at a site, which currently is the Air District for all BAAQMD sites in this report.
Analytical Lab	The agency that weighs particulate filters or does chemical analysis of particulate filters or air samples.
Reporting Agency	The agency that uploads air monitoring data to the EPA's AQS database.
Spatial scale	The relative distance over which the air pollution measurements are representative. Choices are micro, middle, neighborhood, urban, regional, national, or global scales.
Monitor start date	The date valid data collection began for that pollutant at an air monitoring station.
Current Sampling frequency	This reflects the sampling frequency used for district monitors in 2016. This frequency describes if the monitor is operated continuously or intermittently. Intermittent sampling for particulate matter (PM <sub>2.5</sub> , PM <sub>10</sub> , PM <sub>10</sub> -Pb, and TSP-Pb) and toxics is performed by collecting a sample (filter, air canister or other) either every day, every 3 <sup>rd</sup> day, every 6 <sup>th</sup> day or every 12 <sup>th</sup> day (1:1, 1:3, 1:6, 1:12). Samples are subsequently analyzed for the pollutant of interest, for example, PM <sub>2.5</sub> mass or lead concentrations. The Air District at times elects to operate a monitor more frequently than is required. For more information about how the current sampling frequency compares to the required sampling frequency, see the sections on minimum monitoring requirements for that pollutant.
Sampling season	The date range (season) monitors were operated during 2016. While California has a required yearlong O <sub>3</sub> season, EPA has granted a waiver to the Air District so that some ozone sites in the Bay Area are not required to run during the winter.
Probe height (meters)	40 CFR Part 58 Appendix E, 2.0: requires that probe height be 2-15 meters above ground level (AGL).
Distance from supporting structure (meters)	40 CFR Part 58 Appendix E, 2.0: requires the probe be at least 1 meter vertically or horizontally away from any supporting structure unless it is a roof, in which case 1 meter separation is required.

Site or Monitor Information	Definition of Terms
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	40 CFR Part 58 Appendix E, 4.0: requires that the distance from the obstacle to the probe or inlet must be at least twice the height that the obstacle protrudes above the probe or inlet. PM samplers must have a 2 meter separation from walls, parapets and structures.
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	40 CFR Part 58 Appendix E, 4.0: requires that the distance from the obstacle to the probe or inlet must be at least twice the height that the obstacle protrudes above the probe or inlet.
Distance from trees (meters)	40 CFR Part 58 Appendix E, 5.0: requires that probe be at least 10 meters from the nearest tree drip line.
Distance to furnace or incinerator flue (meters)	40 CFR Part 58 Appendix E, 3.0: requires that scavenging be minimized by keeping the probe away from furnace or incineration flues or other minor sources of SO <sub>2</sub> or NO <sub>x</sub> . The separation distance should take into account the heights of the flues, type of waste or fuel burned, and the sulfur content of the fuel.
Distance between monitors fulfilling a QA collocation requirement (meters)	Collocated PM <sub>2.5</sub> , PM <sub>10</sub> , and Pb monitors must be 2-4 meters apart for flow rates >200L/m and 1-4 meters apart for flow rates <200 L/m (40 CFR 58, Appendix A 3.2.3.4(c), 3.3.4.1(c), and 3.4.4.2(b)).
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	40 CFR Part 58, Appendix A 3.2.3.4(c), 3.3.4.1(c), and 3.4.4.2(b) require that PM monitors with flow rates <200L/m have at least a 1 meter separation.
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	40 CFR Part 58, Appendix A 3.2.3.4(c), 3.3.4.1(c), and 3.4.4.2(b) require that PM monitors with flow rates > 200L/m have at least a 2 meter separation.
Unrestricted airflow (degrees)	40 CFR Part 58 Appendix E, 4.0: requires the probe or inlet to have unrestricted airflow in an arc of at least 180 degrees. This arc must include the predominant wind direction for the season of greatest pollutant concentration potential.
Probe material for reactive gases	40 CFR Part 58, Appendix E, 9.0: requires that either Pyrex glass or FEP Teflon be used for intake sampling lines.
Residence time for reactive gases (seconds)	40 CFR Part 58, Appendix E, 9.0: requires a residence time of 20 seconds or less for reactive gas monitors.
Will there be changes within the next 18 months?	Describes if any changes are expected to occur to that monitor at that station within the next 18 months.

Site or Monitor Information	Definition of Terms
Is it suitable for comparison against the annual PM <sub>2.5</sub> ?	40 CFR 58.30: PM <sub>2.5</sub> data from monitors that are located at relatively unique micro-scale, localized hot spot, or unique middle-scale impact sites, and do not represent area-wide concentrations, are not eligible for comparison to the Annual PM <sub>2.5</sub> NAAQS (they are eligible for comparison to the 24-hour PM <sub>2.5</sub> NAAQS). Currently, all of the PM <sub>2.5</sub> sites in the Bay Area are considered to be representative of area-wide concentrations.
Frequency of flow rate verification for PM samplers	40 CFR Part 58, Appendix A, Sections 3.2.1, 3.3.1, 3.3.2, 3.4.1, 3.4.2: require that a one-point flow rate verification check must be performed at least once every month for low-volume PM samplers and quarterly for hi-volume PM samplers.
Frequency of one-point QC check for gaseous instruments	40 CFR Part 58 Appendix A, 3.1.1: requires that QC checks be performed at least once every two weeks.
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	40 CFR Part 58 Appendix A, 3.1.2: requires that SO <sub>2</sub> , CO, O <sub>3</sub> , and NO <sub>2</sub> monitors have annual performance evaluations.
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	40 CFR Part 58 Appendix A, Sections 3.2.2, 3.3.3, 3.4.3: require that PM samplers have flow rate checks every six months.

#### **4. DETAILED STATION INFORMATION FOR SLAMS AND SPM SITES**

#### 4.1 Berkeley Aquatic Park (near-road)

Station Information for Berkeley Aquatic Park	
AQS ID	06-001-0013
GPS coordinates	37.864767, -122.302741
Location	Trailer within 50m east of Interstate 80
Address	1 Bolivar, Berkeley CA 94710
County	Alameda
Distance to road from gaseous probe (meters)	I-80: 8 University Ave: 250
Traffic count (AADT, year)	I-80: 280,400 (2017) University Ave: 18,800 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Gravel, grass, small plants.
Statistical Area	San Francisco-Oakland-Hayward CBSA

This site is monitoring NO/NO<sub>2</sub>, CO, O<sub>3</sub>, PM<sub>2.5</sub>, Ultrafine Particulate Matter (UFP), black carbon (BC) and toxics. Monitoring began on July 1, 2016. The site is located near the city of Berkeley, with a population of 112,580 per the 2010 census.

PM<sub>2.5</sub> monitoring at this site is considered representative of area-wide concentrations within this region even though it is a microscale site. The site type for NO/NO<sub>2</sub>, CO, O<sub>3</sub>, and PM<sub>2.5</sub> in AQS and in the accompanying tables is source oriented and population oriented.

Toxic compounds are determined from canister samples taken at Bethel Island on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded one exceedance of the national 1-hour NO<sub>2</sub> standard and 20 exceedances of the national 24-hour PM<sub>2.5</sub> standard. There were no exceedances of the national standards for O<sub>3</sub>, PM<sub>10</sub>, SO<sub>2</sub>, or CO.



## Berkeley Aquatic Park Monitor Information

Pollutant, POC	O3, 1	NO2, 1	CO, 1	PM2.5, 3
Primary/QA Collocated/Other Parameter code	N/A 44201	Primary 42602	N/A 42101	Primary 88101
Basic monitoring objective(s)	Public Information	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented & Source Oriented	Population Oriented & Source Oriented	Population Oriented & Source Oriented
Monitor type(s)	SPM	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	Near Road	Near Road	Near Road
Instrument manufacturer and model	TECO 49c	TECO 42i	TECO 48i	Met One FEM BAM 1020
Method code	047	074	054	170
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Micro	Micro	Micro	Micro
Monitor start date	07/01/2016	07/01/2016	07/01/2016	07/01/2016
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	6	6	6	5
Distance from supporting structure (meters)	> 1	> 1	> 1	> 2
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	4, 0	4, 0	4, 0	5, 0.75
Distance from trees (meters)	25	25	25	25
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	N/A	N/A	N
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	N/A
Residence time for reactive gases (seconds)	17	19	19	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A	Y
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	Bi-weekly
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/08/2019 08/23/2019	03/08/2019 08/23/2019	03/08/2019 08/23/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	03/08/2019 06/18/2019 09/23/2019 11/15/2019

## Berkeley Aquatic Park Monitor Information

Pollutant, POC	BC, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	N/A
Parameter code	84313	See toxics section
Basic monitoring objective(s)	Research	Research
Site type(s)	Population Oriented & Source Oriented	Population Oriented
Monitor type(s)	SPM	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Teledyne API model 633	Xontech 910A
Method code	894	210
FRM/FEM/ARM/other	N/A	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Micro	Urban
Monitor start date	07/01/2016	07/23/2016
Current Sampling frequency	Continuous	1:12
Sampling season	01/01-12/31	01/01 – 12/31
Probe height (meters)	4	5
Distance from supporting structure (meters)	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	6, 1	4, 0
Distance from trees (meters)	25	25
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A

## 4.2 Bethel Island

Station Information for Bethel Island	
AQS ID	06-013-1002
GPS coordinates	38.006311, -121.641918
Location	Trailer in parking lot
Address	5551 Bethel Island Rd, Bethel Island, CA 94511
County	Contra Costa
Distance to road from gaseous probe (meters)	Bethel Island Rd: 63 Sandmound Blvd: 110
Traffic count (AADT, year)	Bethel Island Rd: 13,050 (2010) Sandmound Blvd: 4,270 (2010) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Gravel surrounded by grassy fields
Statistical Area	San Francisco-Oakland-Hayward CBSA

The site is 26 miles east of the only sea-level gap (the Carquinez Strait) between the two regions. The town of Bethel Island, 0.6 miles to the north, has a population of 2,137 according to the 2010 census. This site was operated by the California Air Resources Board (CARB) from 1981 until late 1986 and by the Air District from then on.

Ozone and NO/NO<sub>2</sub> are measured because the area is in the transport corridor between the San Francisco Bay Area and the Central Valley, both of which are major sources of ozone, ozone precursors, and particulates. Traffic volume near the site is low, so CO measurements tend to be representative of natural background levels, or regional transport. SO<sub>2</sub> is measured because the area is downwind from numerous refineries, which can be large sources of SO<sub>2</sub>. PM<sub>10</sub> is measured because easterly winds occasionally transport particulates from the Central Valley, and because the filters can be analyzed to determine sulfate and nitrate levels transported from the Central Valley.

Toxic compounds are determined from canister samples taken at Bethel Island on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

PM<sub>10</sub> monitoring was changed from 1:6 to 1:12 sampling effective January 1, 2013 to accommodate limited resources. Because the Bay Area is well above the minimum monitoring requirements for PM<sub>10</sub>, EPA approved this decrease in sampling frequency as well as converting these PM<sub>10</sub> monitors from SLAMS to SPMs. Therefore, this monitor is no longer counted in PM<sub>10</sub> minimum monitoring requirements.

During the most recent three years, this site recorded three exceedances of the national 70 ppb 8-hour ozone standard and no exceedances of the national standards for NO<sub>2</sub>, PM<sub>10</sub>, SO<sub>2</sub>, or CO.

### Bethel Island Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Regional Transport & Highest Conc.	General Background	Regional Transport
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Urban	Urban	Urban
Monitor start date	03/01/1981	03/01/1981	03/01/1981
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	7	7	7
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	13	13	13
Distance to furnace or incinerator flue (meters)	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	15	16	17
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/08/2019 11/14/2019	05/08/2019 11/14/2019	05/08/2019 11/14/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## Bethel Island Monitor Information

Pollutant, POC	SO2, 1	PM10, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	Primary	N/A
Parameter code	42401	81102	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Regional Transport	Regional Transport	General / Background
Monitor type(s)	SLAMS	SPM	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 43i	Andersen GUV-16HBLA	Xontech 901
Method code	060	063	210
FRM/FEM/ARM/other	FEM	FRM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	Air District	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Urban	Neighborhood	Neighborhood
Monitor start date	03/01/1981	11/05/1986	03/27/1998
Current Sampling frequency	Continuous	1:12	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	7	5	6
Distance from supporting structure (meters)	> 1	>2	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	13	14	13
Distance to furnace or incinerator flue (meters)	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	N/A	Glass
Residence time for reactive gases (seconds)	16	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	Quarterly	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/08/2019 11/14/2019	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	02/23/2019, 05/08/2019 07/24/2019, 11/07/2019	N/A

### 4.3 Concord

Station Information for Concord	
AQS ID	06-013-0002
GPS coordinates	37.936013, -122.026154
Location	One-story commercial building
Address	2956-A Treat Blvd, Concord CA 94518
County	Contra Costa
Distance to road from gaseous probe (meters)	Treat Blvd: 181 Oak Grove Rd: 244
Traffic count (AADT, year)	Treat Blvd: 39,860 (2017) Oak Grove Rd: 24,910 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Concord was chosen for air monitoring because it is the largest city in Contra Costa County, with a population of 122,067 according to the 2010 census. Because Concord is in the Diablo Valley, locally emitted pollutants can become trapped when winds are light. Large emission sources in the valley include the two major freeways, Interstate 680 and California Highway 4, and two refineries at the north end of the valley.

The air monitoring site is in the back of a shopping center, near the intersection of two major streets, and surrounded by residential neighborhoods. There is no industry in the immediate vicinity. NO/NO<sub>2</sub> is measured because of local mobile emissions. Ozone is measured at the site because hot, inland summertime temperatures combined with precursor pollutants stagnating in the surrounding valley often produces high ozone levels. Carbon monoxide is measured because the site is near two major roads, Treat Blvd. and Oak Grove Road. SO<sub>2</sub> is measured because the site is six miles south of the Tesoro and the Shell Refineries, both potential major sources of SO<sub>2</sub>. PM<sub>10</sub> and PM<sub>2.5</sub> are measured because light winds combined with surface-based inversions during the winter months can cause elevated particulate levels in the valley.

PM<sub>10</sub> monitoring was changed from 1:6 to 1:12 sampling effective January 1, 2013 to accommodate limited resources. Because the Bay Area is well above the minimum monitoring requirements for PM<sub>10</sub>, EPA approved this decrease in sampling frequency as well as converting these PM<sub>10</sub> monitors from SLAMS to SPMs. Therefore, this monitor is no longer counted in PM<sub>10</sub> minimum monitoring requirements.

Toxic compounds are determined from canister samples taken at Concord on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded two exceedances of the national 70 ppb 8-hour ozone standard, and 20 exceedances of the national 24-hour PM<sub>2.5</sub> standard. No exceedances of the national standards for PM<sub>10</sub>, NO<sub>2</sub>, SO<sub>2</sub>, or CO were measured during the last three years.

## Concord Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1	SO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary	N/A
Parameter code	44201	42101	42601 / 42602	42401
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented & Source Impact
Monitor type(s)	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i	TECO 43i
Method code	047	054	074	060
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Neighborhood
Monitor start date	04/09/1980	02/21/1980	2/21/1980	02/21/1980
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	9	9	9	9
Distance from supporting structure (meters)	> 1	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	24	24	24	24
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	9	10	10	10
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	02/07/2019 07/23/2019	02/07/2019 07/23/2019	02/07/2019 07/23/2019	02/07/2019 07/23/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A



## Concord Monitor Information

Pollutant, POC	PM10, 1	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	Primary	N/A
Parameter code	81102	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented & Highest Conc.	Population Oriented & Source Impact
Monitor type(s)	SPM	SLAMS	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	Andersen HiVol 1200	Met One BAM 1020	Xontech 901
Method code	063	170	210
FRM/FEM/ARM/other	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	N/A	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Urban	Urban	Urban
Monitor start date	11/04/1986	1/1/2013	08/08/1989
Current Sampling frequency	1:12	Continuous	1:12
Sampling season	01/01-12/31	01/01-12/31	01/01 - 12/31
Probe height (meters)	6	6	9
Distance from supporting structure (meters)	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	15	22	24
Distance to furnace or incinerator flue (meters)	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/06/2019, 04/18/2019 07/22/2019, 10/17/2019	02/06/2019, 04/18/2019 07/22/2019, 10/17/2019	N/A

#### 4.4 Crockett

Station Information for Crockett	
AQS ID	06-013-1001
GPS coordinates	38.054920, -122.233229
Location	Pump house
Address	End of Kendall Avenue, Crockett CA 94525
County	Contra Costa
Distance to road from gaseous probe (meters)	San Pablo Ave: 68
Traffic count (AADT, year)	San Pablo Ave: 2,797 (2013) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Vegetative
Statistical Area	San Francisco-Oakland-Hayward CBSA

Crockett was chosen for SO<sub>2</sub> source-oriented monitoring because it is downwind of the Phillips 66 Refinery. Prevailing winds in the area are from the west, which transport SO<sub>2</sub> emissions from the refinery over the town of Crockett, a predominately residential community with a population of 3,094 according to the 2010 census. The monitoring site is located on the west side of Crockett 0.9 miles northeast of the refinery boundary. The only other major industry near Crockett is C&H Sugar, which is not a significant source of SO<sub>2</sub> emissions.

VOC toxic compounds are sampled at Crockett on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

Crockett is classified as an SPM site. EPA siting criteria require the probe be located at least 10 meters from the drip line of all trees within the 180-degree arc of unrestricted airflow for source-oriented monitoring as determined by the predominant wind direction and the direction of the refinery. The closest tree drip line within the 180-degree arc is less than 10 meters from the probe, which does not meet siting criteria. The Air District has been unable to negotiate with the local homeowner's association for the removal of this tree. Even though the siting criteria for a SLAMS site cannot be met, the site is still suitable for source-oriented monitoring as an SPM site.

SO<sub>2</sub> concentrations measured at Crockett did not exceed the national 1-hour 75 ppb standard during the last three years.

## Crockett Monitor Information

Pollutant, POC	SO2, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	N/A
Parameter code	42401	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Research
Site type(s)	Population Oriented & Source Oriented	Population Oriented & Source Oriented
Monitor type(s)	SPM	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	TECO 43i	Xontech 901
Method code	060	210
FRM/FEM/ARM/other	FEM	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Urban
Monitor start date	01/01/1979	06/05/1999
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 - 12/31
Probe height (meters)	6	6
Distance from supporting structure (meters)	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	1	1
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	270	270
Probe material for reactive gases	Teflon	Glass
Residence time for reactive gases (seconds)	11	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/08/2019 10/07/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A

## 4.5 Fairfield

Station Information for Fairfield	
AQS ID	06-095-0005
GPS coordinates	38.227066, -122.075624
Location	Small trailer in open field
Address	1010 Chadbourne Rd, Fairfield, CA 94534
County	Solano
Distance to road from gaseous probe (meters)	Cordelia Rd: 194 Chadbourne Rd: 705
Traffic count (AADT, year)	Cordelia Rd: 4,819 (2013) Chadbourne Rd: 3,674 (2013) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Vegetative
Statistic Area	Vallejo-Fairfield CBSA

Fairfield lies in the northeast part of the Air District in the Carquinez Strait Region, the only sea level gap between the Bay Area and the Central Valley. Prevailing westerly winds carry ozone and its precursors from the Bay Area to the Sacramento Valley.

The monitoring site is in a rural area between Fairfield/Suisun City and the greater Bay Area. Prevailing winds are westerly during the summer season. Therefore, the monitor normally measures ozone concentrations coming from the Bay Area. Occasionally easterly winds transport ozone from the Central Valley to Fairfield and the Bay Area.

Over the past decade the Fairfield/Suisun City area has grown considerably. According to the 2010 census the area has a combined population of 138,815, the largest urban area in Solano County. Thus, Fairfield is also a population-oriented ozone monitoring site.

Ozone concentrations measured at Fairfield did not exceed the national 70 ppb 8-hour ozone standard during the last three years.

## Fairfield Monitor Information

Pollutant, POC	O3, 1
Primary/QA Collocated/Other	N/A
Parameter code	44201
Basic monitoring objective(s)	NAAQS comparison
Site type(s)	Population Oriented & Regional Transport
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 49i
Method code	047
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Urban
Monitor start date	05/29/2002
Current Sampling frequency	Continuous
Sampling season	01/01 - 12/31
Probe height (meters)	4
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	> 50
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	4
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/22/2019 04/02/2019 07/03/2019 10/08/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

## 4.6 Forest Knolls

Station Information for Forest Knolls	
AQS ID	06-041-2001
GPS coordinates	38.015136, -122.689531
Location	Roof
Address	6 Castro Street, Forest Knolls, CA 94933
County	Marin
Distance to road from probe (meters)	Sir Francis Drake Blvd at Mountain View: 902 Sir Francis Drake Blvd at Montezuma Road: 18 Castro St: 13 Montezuma Road: 55
Traffic count (AADT, year)	Sir Francis Drake Blvd at Montezuma Road: 4,300 (est. 2019) Castro St: <150 (est. 2019) Montezuma Road: <500 (est. 2019) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistic Area	San Francisco-Oakland-Hayward CBSA

Forest Knolls was chosen for monitoring black carbon (BC) due to community interest about wood smoke in the San Geronimo Valley and to better understand and characterize the wood smoke source category in sheltered valley locations where winter wood burning often is the primary source of home heating. Lagunitas-Forest Knolls is considered a Census Designated Place (CDP) with a population of 1,819 based on the 2010 census.

Forest Knolls is located in San Geronimo Valley about 10 miles west to northwest of San Rafael. Wintertime meteorological conditions are frequently conducive to trapping wood smoke in the valley, particularly during cold, still evenings. Many of the homes do not have residential gas for heating and, therefore, burn wood.

## Forest Knolls Monitor Information

Pollutant, POC	BC, 1
Primary/QA Collocated/Other	N/A
Parameter code	84313
Basic monitoring objective(s)	Research
Site type(s)	Population Oriented
Monitor type(s)	SPM
Network affiliation(s)	N/A
Instrument manufacturer and model	Teledyne API AE-633
Method code	894
FRM/FEM/ARM/other	N/A
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Neighborhood
Monitor start date	01/16/2013
Current Sampling frequency	Continuous
Sampling season	01/01-12/31
Probe height (meters)	5
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	4
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	N/A
Residence time for reactive gases (seconds)	N/A
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

## 4.7 Fort Cronkhite

Station Information for Fort Cronkhite	
AQS ID	06-041-0004
GPS coordinates	37.832725, -122.527658
Location	At ground level behind a ranger residence
Address	Building 1111, Fort Cronkhite, Sausalito CA 94965
County	Marin
Distance to road from probe (meters)	Bunker Road: 16
Traffic count (AADT, year)	Bunker Road: 1039 (2018) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Vegetative
Statistical Area	San Francisco-Oakland-Hayward CBSA

Fort Cronkhite was chosen as a monitoring site because it is representative of background levels of VOC toxics compounds transported into the Bay Area from the Pacific Ocean due to prevailing westerly winds. The site is 0.5 miles east of the Pacific Ocean, on the north side of the Golden Gate gap which opens into San Francisco Bay. The monitor is located within the Golden Gate National Recreation Area (GGNRA) near the visitor center at Fort Cronkhite. Low concentrations of toxics from this site provide a baseline to compare other toxics measurements in the Bay Area.

Toxics concentrations measured at this site may reflect some anthropogenic sources in addition to natural background sources such as VOC toxics contributions from ships headed to and from the Bay Area and Central Valley ports, and from ships sailing along the coast. Additionally, there can be a small contribution from vehicle traffic in areas upwind of the site within the GGNRA. Despite these contributions, when winds are from the west, the VOC toxics levels at this site reflect the lowest levels in the Bay Area.

The closest industrial sources are in San Francisco about eight miles southeast of the site. The closest towns are Sausalito, three miles to the east-northeast with a population of 7,061, and Marin City, three miles to the northeast with a population of 2,666 based on the 2010 census. Sausalito and Marin City have little impact on the monitoring site because winds are typically from the west so the site is upwind of these towns, and the towns have no significant industrial sources.

Toxic compounds are determined from canister samples taken at Fort Cronkhite on a 1:12 schedule and later analyzed in the Air District laboratory. More information



about the toxics monitoring program can be found in the Toxics Program section of this report.

### Fort Cronkhite Monitor Information

Pollutant, POC	Toxics, 3
Primary/QA Collocated/Other	N/A
Parameter code	See toxics section
Basic monitoring objective(s)	Research
Site type(s)	General / Background
Monitor type(s)	SPM
Network affiliation(s)	N/A
Instrument manufacturer and model	Xontech 910A
Method code	210
FRM/FEM/ARM/other	N/A
Collecting Agency	Air District
Analytical Lab	Air District
Reporting Agency	Air District
Spatial scale	Regional
Monitor start date	03/26/1987
Current Sampling frequency	1:12
Sampling season	01/01 - 12/31
Probe height (meters)	7
Distance from supporting structure (meters)	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	20
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Glass
Residence time for reactive gases (seconds)	N/A
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

## 4.8 Gilroy

Station Information for Gilroy	
AQS ID	06-085-0002
GPS coordinates	36.999571, -121.574684
Location	Air monitoring shelter next to water pump station
Address	9 <sup>th</sup> and Princevalle St, Gilroy, CA 95020
County	Santa Clara
Distance to road from gaseous probe (meters)	Princevalle St: 18 9 <sup>th</sup> St: 16 8 <sup>th</sup> St.: 142 10 <sup>th</sup> St: 185
Traffic count (AADT, year)	Princevalle St: 3,627 (2018) 9 <sup>th</sup> St: 1,386 (2019) 8 <sup>th</sup> St.: 2,574 (2019) 10 <sup>th</sup> St: 12,700 (2008) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

Prevailing northwesterly afternoon winds carry ozone and ozone precursors from the San Jose area southward through the Santa Clara Valley. When temperatures are hot, and solar insolation is strong, these precursors react and can form high concentrations of ozone in the Gilroy area. As Gilroy grew in population (48,821 according to the 2010 census) the site was considered not only a regional ozone transport site but also a population-oriented ozone site. PM<sub>2.5</sub> is measured because light winds combined with surface-based inversions during the winter months can cause elevated particulate levels in the valley.

The monitoring site is in a residential area of Gilroy on the west side of the Santa Clara Valley.

During the most recent three years, this site recorded one exceedance of the national 70 ppb 8-hour ozone standard and 14 exceedances of the national 24-hour PM<sub>2.5</sub> standard.

## Gilroy Monitor Information

Pollutant, POC	O3, 1	PM2.5, 3
Primary/QA Collocated/Other	N/A	Primary
Parameter code	44201	88101
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented & Regional Transport	Population Oriented & Regional Transport
Monitor type(s)	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	TECO 49i	Met One FEM BAM 1020
Method code	047	170
FRM/FEM/ARM/other	FEM	FEM
Collecting Agency	Air District	Air District
Analytical Lab	N/A	N/A
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Neighborhood
Monitor start date	07/01/1980	10/31/2009
Current Sampling frequency	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	5	4
Distance from supporting structure (meters)	>1	No supporting structure / ground level
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	N/A
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A	1.8 <sup>a</sup>
Distance from trees (meters)	26	26
Distance to furnace or incinerator flue (meters)	14	14
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	Teflon	N/A
Residence time for reactive gases (seconds)	14	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y
Frequency of flow rate verification for PM samplers	N/A	Bi-weekly
Frequency of one-point QC check for gaseous instruments	Every other day	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/24/2019, 04/03/2019 07/10/2019, 10/02/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	01/24/2019, 04/03/2019 07/10/2019, 10/02/2019

- a The PM<sub>2.5</sub> monitor is outdoors, ground based. The probe is 4m above ground. A nearby shelter is 1.8m away and is the eve of the shelter is 0.12m above the probe height. This is not an obstruction because the probe is more than twice the distance that the eve extends above the probe. The shelter has a slanted roof that peaks at a height of 3.99m. The probe is 3.9m away from the roof peak, which is 0.99m above the probe. This is not an obstruction because the probe is more than twice the distance that the roof peak extends above the probe.

## 4.9 Hayward

Station Information for Hayward	
AQS ID	06-001-2001
GPS coordinates	37.654456, -122.031547
Location	Pump house near water tank
Address	3466 La Mesa Drive, Hayward, CA 94542
County	Alameda
Distance to road from gaseous probe (meters)	Hayward Blvd: 26 La Mesa Dr: 38 Farmhill Drive: 205
Traffic count (AADT, year)	Hayward Blvd: 4,293 (2010) La Mesa Drive: 500 (2007) Farmhill Drive: 2,500 (<2006) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

The city of Hayward has a population of 144,186 according to the 2010 census. Located on the east side of Hayward at an elevation of 951 feet, it is the highest elevation ozone SLAMS in the Air District. Studies had shown that on high ozone days, a cloud of ozone and ozone precursors moves southward from Oakland on the west side of the East Bay Hills.

Because ozone monitoring sites were typically located in the low-lying areas of the East and South Bay, i.e., in Oakland and San Jose, this site was chosen to be between them, but at a higher elevation. Thus, the site gives an indication of ozone levels aloft and sub-regional transport. The Hayward site is also important because it provides air quality forecasting information concerning residual ozone from the previous day. Although there is a large water tank onsite in the upwind direction, the instrument probe is high enough so that the tank is not an obstacle.

During the most recent three years, this site recorded five exceedances of the national 70 ppb 8-hour ozone standard.

## Hayward Monitor Information

Pollutant, POC	O3, 1
Primary/QA Collocated/Other	N/A
Parameter code	44201
Basic monitoring objective(s)	NAAQS comparison & Research
Site type(s)	Other (Sub-Regional Transport)
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 49i
Method code	047
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Urban
Monitor start date	05/31/1977
Current Sampling frequency	Continuous
Sampling season	01/01-12/31
Probe height (meters)	7
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	11
Distance to furnace or incinerator flue (meters)	N/A
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	16
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Every other day
	01/23/2019
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/09/2019
	07/08/2019
	10/04/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

#### 4.10 Laney College (near-road)

Station Information for Laney College	
AQS ID	06-001-0012
GPS coordinates	37.793624, -122.263376
Location	Trailer east of Interstate 880
Address	Laney College 8 <sup>th</sup> St. parking lot, Aisle J, Oakland, CA 94607
County	Alameda
Distance to road from gaseous probe (meters)	I-880: 20 8 <sup>th</sup> St: 116 Fallon St: 130 5 <sup>th</sup> Ave: 419
Traffic count (AADT, year)	Interstate 880: 219,000 (2017) 8 <sup>th</sup> St: 16,055 (2012) Fallon St: 4,000 (2014) 5 <sup>th</sup> Ave: <5,000 (2014) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

The Air District began monitoring pollutants at this site on February 1, 2014. The site is along a segment of roadway with the second highest Fleet Equivalent AADT (FE-AADT) in the Bay Area. The roadway segment with the highest FE-AADT in the Bay Area was not suitable for monitoring because it was near train tracks and no access was permitted across the easement by the land owner (Union Pacific) due to safety concerns. The site is in Oakland which is the largest city in Alameda County, with a population of 390,724 according to the 2010 census.

This site monitors NO/NO<sub>2</sub>, CO, and PM<sub>2.5</sub>, Ultrafine Particulate Matter (UFP), black carbon (BC) and toxics. PM<sub>2.5</sub> monitoring at this site is considered representative of area-wide concentrations within this major metropolitan region.

Toxic compounds are determined from canister samples taken at Laney College on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

The site type for NO/NO<sub>2</sub>, CO, and PM<sub>2.5</sub> in AQS and in the accompanying tables is source oriented and population oriented. The site is within 0.25 miles of residential and commercial areas in Oakland.

During the most recent three years, this site recorded 22 exceedances of the national 24-hour PM<sub>2.5</sub> standard. There were no exceedances of the national standards for NO<sub>2</sub> or CO.

## Laney College Monitor Information

Pollutant, POC	NO2, 1	CO, 1	PM2.5, 3	BC, 1	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A	Primary	N/A	N/A
Parameter code	42601 / 42602	42101	88101	84313	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	Public Information	Research
Site type(s)	Source Impact & Population Oriented	Source Impact & Population Oriented	Source Impact & Population Oriented	Source Impact	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SPM	SPM
Network affiliation(s)	Near Road	Near Road	Near Road	N/A	N/A
Instrument manufacturer and model	TECO 42i	TECO 48i	Met One FEM BAM 1020	Teledyne API AE-633	Xontech 901
Method code	074	054	170	894	210
FRM/FEM/ARM/other	FRM	FRM	FEM	N/A	N/A
Collecting Agency	Air District	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A	Air District
Reporting Agency	Air District	Air District	Air District	Air District	Air District
Spatial scale	Micro	Micro	Micro	Micro	Urban
Monitor start date	02/01/2014	02/01/2014	02/01/2014	02/01/2014	02/04/2014
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01-12/31	01/01 – 12/31
Probe height (meters)	6	6	5	5	5
Distance from supporting structure (meters)	>1	>1	>2	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None	None
Distance from trees (meters)	None	None	None	None	None
Distance to furnace or incinerator flue (meters)	None	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	N/A	N/A	Glass
Residence time for reactive gases (seconds)	16	16	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	Y	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	Bi-weekly	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	N/A	N/A	N/A
Dates of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/12/2019 09/11/2019	03/12/2019 09/11/2019	N/A	N/A	N/A
Date of semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	03/12/2019 06/18/2019 09/11/2019 11/15/2019	N/A	N/A



## 4.11 Livermore

Station Information for Livermore	
AQS ID	06-001-0007
GPS coordinates	37.687526, -121.784217
Location	One-story commercial building
Address	793 Rincon Avenue, Livermore, CA 94551
County	Alameda
Distance to road from gaseous probe (meters)	Rincon Ave: 68 Pine St: 95 Interstate 580: 1,320 Portola Ave: 722
Traffic count (AADT, year)	Rincon Ave: 3,091 (2013)    Portola Ave: 21,747 (2016) Pine St: 4,263 (2013)    Interstate 580: 202,000 (2016) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Past measurements have shown this area to have the highest ozone levels in the Bay Area. Livermore is located within the Livermore Valley, an east-west oriented inland valley between the San Francisco Bay and the Central Valley. Wind analyses of high ozone days show ozone precursors moving to this valley from the Hayward and Niles Canyon Gaps to the west, and from the San Ramon Valley to the north. The air monitoring site is west of the city center, in a residential neighborhood. The station is in a small one-story shopping center, with a little-used parking lot in front of the station and a city park behind it.

There are no industrial sources in the immediate vicinity of the site. Ozone and its precursors and NO/NO<sub>2</sub>, are measured because the area is downwind of large sources of ozone precursors. PM<sub>2.5</sub> is measured because light winds combined with surface-based inversions during the winter months can cause elevated particulate levels. Black carbon (BC) is measured to better determine the composition and relationship between BC and PM<sub>2.5</sub>.

VOC toxic compounds are sampled at Livermore on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

The Livermore site is part of an unofficial Photochemical Assessment Monitoring Stations (PAMS) program. This is a program to measure hourly speciated hydrocarbons

using a gas chromatograph analyzer at two Bay Area locations. The other location is in San Ramon. A full description of the PAMS program can be found in the PAMS section of this document. As part of the 2015 O<sub>3</sub> NAAQS revision, EPA updated the PAMS requirements. Starting in 2019, PAMS measurements are required at NCore sites that are located in Core-Based Statistical Areas (CBSAs) with populations of 1,000,000 or more. The EPA approved the Air District's request to conduct PAMS monitoring at Livermore (see APPENDIX F). Under this approval, NO<sub>y</sub> will stop at San Jose and will begin at Livermore in 2019. As of May 20, 2019, San Jose is still collecting NO<sub>y</sub> data until NO<sub>y</sub> is added to the Livermore PAMS site.

During the most recent three years, this site recorded 16 exceedances of the national 70 ppb 8-hour ozone standard, 16 exceedances of the national 24-hour PM<sub>2.5</sub> standard, and no exceedances of the national NO<sub>2</sub> standard.

## Livermore Monitor Information

Pollutant, POC	O3, 1	NO2, 1	PM2.5, 3
Primary/QA Collocated/Other	N/A	Primary	Primary
Parameter code	44201	42601 / 42602	88101
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison & Research	NAAQS comparison
Site type(s)	Population Oriented, Highest Concentration	Population Oriented	Population Oriented & Highest Conc.
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	Unofficial PAMS	Unofficial PAMS	N/A
Instrument manufacturer and model	TECO 49i	TECO 42i	Met One FEM BAM 1020
Method code	047	074	170
FRM/FEM/ARM/other	FEM	FRM	FEM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	Air District	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	01/01/2000	12/31/1999	03/01/2011
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	6	6	5
Distance from supporting structure (meters)	> 1	> 1	> 2
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	51	51	52
Distance to furnace or incinerator flue (meters)	17	17	21
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	N/A
Residence time for reactive gases (seconds)	13	13	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	Y
Frequency of flow rate verification for PM samplers	N/A	N/A	Bi-weekly
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	02/28/2019 08/07/2019 11/04/2019	02/28/2019 08/07/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	02/28/2019, 05/23/2019 08/06/2019, 11/04/2019

## Livermore Monitor Information

Pollutant, POC	Speciated PM2.5, 5	BC, 1	Toxics, 3
Primary/QA Collocated/Other	Other	N/A	N/A
Parameter code	88502 (pm mass) – many others see Section 5.5.1	84313	See toxics section
Basic monitoring objective(s)	Research	Research	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SPM	SPM	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	Met One SASS	Teledyne API AE-633	Xontech 901
Method code	810	894	210
FRM/FEM/ARM/other	N/A	N/A	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	N/A	Air District
Reporting Agency	N/A	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	06/11/2008	01/01/2012	01/11/2000
Current Sampling frequency	1:6	Continuous	1:12
Sampling season	01/01 - 12/31	01/01-12/31	01/01 - 12/31
Probe height (meters)	5	6	6
Distance from supporting structure (meters)	>2	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	55	52	51
Distance to furnace or incinerator flue (meters)	17	17	17
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	270
Probe material for reactive gases	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N	N/A	N/A
Frequency of flow rate verification for PM samplers	Monthly	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/28/2019, 05/23/2019, 11/04/2019	N/A	N/A

## 4.12 Los Gatos

Station Information for Los Gatos	
AQS ID	06-085-1001
GPS coordinates	37.226862, -121.979675
Location	Top of fire station's hose drying tower
Address	306 University Ave, Los Gatos, CA 95030
County	Santa Clara
Distance to road From gaseous probe (meters)	University Ave: 37 Bentley Ave: 27 State Route 17: 291 State Route 9: 121
Traffic count (AADT, year)	University Ave: 13,000 (2016) Bentley Ave: 1,000 (2020) State Route 17: 97,000 (2017) State Route 9: 34,700 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

Los Gatos was chosen for ozone monitoring because prevailing northerly winds transport ozone and ozone precursors from the densely populated area around the south Bay Area to the west side of the Santa Clara Valley.

High ozone levels are in part due to Los Gatos being situated at the base of the Santa Cruz Mountains, which act as a barrier to the movement of polluted air. The monitoring site is located near the downtown area at a fire station surrounded by residential neighborhoods. The city of Los Gatos has a population of 29,413 according to the 2010 census.

During the most recent three years, this site recorded five exceedances of the national 70 ppb 8-hour ozone standard.

## Los Gatos Monitor Information

Pollutant, POC	O3, 1
Primary/QA Collocated/Other	N/A
Parameter code	44201
Basic monitoring objective(s)	NAAQS comparison
Site type(s)	Population Oriented
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 49i
Method code	047
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Neighborhood
Monitor start date	04/01/1972
Current Sampling frequency	Continuous
Sampling season	01/01 - 12/31
Probe height (meters)	11.0
Distance from supporting structure (meters)	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from trees (meters)	16
Distance to furnace or incinerator flue (meters)	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	16
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Daily
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/25/2019 04/10/2019 07/09/2019 10/03/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

#### 4.13 Martinez

Station Information for Martinez	
AQS ID	06-013-2001
GPS coordinates	38.012816, -122.134467
Location	Small sampling shelter next to fire station
Address	521 Jones St, Martinez, CA 94553
County	Contra Costa
Distance to road from gaseous probe (meters)	Jones St: 22 Alhambra Ave: 19
Traffic count (AADT, year)	Jones St: 2,000 (2008) Alhambra Ave: 25,001 (2012) Traffic counts data were updated on April 1, 2020 reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Martinez was chosen for SO<sub>2</sub> source-oriented monitoring because the Shell and Tesoro oil refineries are located in north and east sections of the city. The Carquinez Strait borders the city to the north and the prevailing winds are from the west. However, north and east winds can transport SO<sub>2</sub> emissions from the refineries over populated areas of the city.

The monitoring site is located near downtown Martinez and is 0.5 miles south of the Shell Refinery and 2.5 miles west of the Tesoro Refinery. According to the 2010 census, Martinez has a 2010 population of 35,824. There are no industrial activities or SO<sub>2</sub> sources nearby other than the refineries.

VOC toxic compounds are sampled at Martinez on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

SO<sub>2</sub> concentrations measured at Martinez did not exceed the national 1-hour 75-ppb standard during the last three years.

## Martinez Monitor Information

Pollutant, POC	SO2, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	N/A
Parameter code	42401	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Research
Site type(s)	Population Oriented & Source Impact	Population Oriented
Monitor type(s)	SLAMS	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	TECO 43i	Xontech 901
Method code	060	210
FRM/FEM/ARM/other	FEM	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Neighborhood
Monitor start date	07/02/1973	06/01/2002
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	7	7
Distance from supporting structure (meters)	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	11	11
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	Teflon	Glass
Residence time for reactive gases (seconds)	13	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/10/2019 07/02/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A



#### 4.14 Napa Valley College

Station Information for Napa	
AQS ID	06-055-0004
GPS coordinates	38.278849, -122.275024
Location	Trailer in parking lot
Address	North College Parking, Napa, CA 94558
County	Napa
Distance to road from gaseous probe (meters)	Napa Valley Hwy Rt 221: 100 Imola Ave Rt 121: 200
Traffic count (AADT, year)	Napa Valley Hwy Rt 221: 36,000 (2017) Imola Ave (Route 121): 25,400 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data
Groundcover	Paved
Statistical Area	Napa CBSA

The city is located in the center of Napa Valley where agricultural burning and fireplace usage during the fall and winter can result in high particulate levels. In summer months, Napa can have elevated ozone levels when central Bay Area ozone precursors are transported north to the city. The site was opened on April 1, 2018 as a replacement to the Napa site. The Napa site relocation request and approval correspondence with EPA is in APPENDIX G

The air monitoring site is situated about 2 miles south of downtown Napa in an open space near a mixed residential and commercial neighborhood. There are no industrial sources in the immediate vicinity. Ozone and NO/NO<sub>2</sub> are measured because southerly winds carry ozone and its precursors into Napa.

Carbon monoxide is measured because the Napa Valley is a major tourist attraction with resulting high traffic volumes through the city. Continuous PM<sub>2.5</sub> is measured using an FEM because of agricultural and household wood burning.

VOC toxic compounds are sampled at Napa on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

Since monitoring began on April 1, 2018, this site recorded two exceedances of the national 8-hour ozone standard, and 12 exceedances of the national 24-hour PM<sub>2.5</sub> standard. No exceedances of the national standards for NO<sub>2</sub> or CO were recorded.

## Napa Valley College Monitor Information

Pollutant, POC	O3, 1	NO2, 1	CO, 1
Primary/QA Collocated/Other	Primary	Primary	N/A
Parameter code	44201	42601 / 42602	42101
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49c	TECO 42i	TECO 48i
Method code	047	074	054
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Middle
Monitor start date	04/01/2018	04/01/2018	04/01/2018
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5	5	5
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	12	15	14
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Dates of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/31/2019 07/16/2019	01/31/2019 07/16/2019	01/31/2019 07/16/2019
Date of semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## Napa Valley College Monitor Information

Pollutant, POC	PM10, 1	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	Primary	N/A
Parameter code	81102	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented & Highest Conc.	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	Tisch Env. HiVol TE-60	Met One FEM BAM 1020	Xontech 901
Method code	141	170	210
FRM/FEM/ARM/other	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	N/A	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Middle	Neighborhood	Middle
Monitor start date	09/23/2002	04/01/2018	04/01/2018
Current Sampling frequency	1:6	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	4	5	5
Distance from supporting structure (meters)	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	N/A	N/A	N/A
Distance to furnace or incinerator flue (meters)	N/A	N/A	N/A
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A
Dates of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	01/30/2019 04/22/2019 07/15/2019 10/21/2019	01/30/2019 04/22/2019 07/15/2019 10/21/2019	N/A

## 4.15 Oakland East

Station Information for Oakland East	
AQS ID	06-001-0009
GPS coordinates	37.743065, -122.169935
Location	Two-story commercial building
Address	9925 International Blvd, Oakland, CA 94603
County	Alameda
Distance to road from gaseous probe (meters)	International Blvd: 19 98 <sup>th</sup> St: 43                      99 <sup>th</sup> St: 23
Traffic count (AADT, year)	International Blvd: 21,988 (2011) 98 <sup>th</sup> St: 31,340 (<2006)                      99 <sup>th</sup> St: 100 (2008) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Oakland is an important area for air pollution monitoring because it is the largest city in Alameda County, with a population of 390,724 according to the 2010 census. It has large emission sources within its boundaries, such as a major maritime port, an international airport, extensive areas of industry, and several major freeways. These sources have the potential to emit significant amounts of CO and ozone precursors, as well as particulates and toxic compounds.

The monitoring site is located seven miles southeast of downtown Oakland, on a commercial strip in a residential area. Ozone and NO/NO<sub>2</sub> are measured to monitor population oriented to these pollutants. Carbon monoxide is measured because of the high volume of traffic in the city, which includes several major freeways. PM<sub>2.5</sub> is measured due to the large emission sources in the area, and because light winds combined with wood burning, vehicular traffic, and surface-based inversions during winter can cause elevated particulate concentrations.

The monitoring scale for ozone is middle scale. Following an EPA Region 9 review of the distance between the gaseous probe and the roadway, and the corresponding traffic count, EPA Region 9 suggested this monitor be changed from SLAMS to SPM and the Air District agreed to the change. Consequently, this monitor cannot be used toward meeting the minimum monitoring requirements for ozone.

The PM<sub>2.5</sub> monitor is middle scale based on the distance from the roadway and nearby traffic count. The Air District considers this monitor to represent area-wide air

quality and, therefore, comparable to the NAAQS because the site represents many similar locations throughout the metropolitan area.

VOC toxic compounds are sampled at Oakland East on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, the national 24-hour PM<sub>2.5</sub> standard was exceeded on 20 days, and the national 70 ppb 8-hour ozone standard was exceeded on four days. No exceedances of the national standards for NO<sub>2</sub> or CO were measured during the last three years.

## Oakland East Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	Research	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SPM	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Middle	Middle	Middle
Monitor start date	11/01/2007	11/01/2007	11/01/2007
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	10	10	10
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	21	21	21
Distance to furnace or incinerator flue (meters)	8	8	8
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	15	16	16
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/30/2019 11/13/2019	04/30/2019 11/13/2019	04/30/2019 11/13/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## Oakland East Monitor Information

Pollutant, POC	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A
Parameter code	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Met One FEM BAM 1020	Xontech 901
Method code	170	210
FRM/FEM/ARM/other	FEM	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Middle	Middle
Monitor start date	10/01/2009	11/01/2007
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	7	9
Distance from supporting structure (meters)	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	21	21
Distance to furnace or incinerator flue (meters)	5	8
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	Y	N/A
Frequency of flow rate verification for PM samplers	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/19/2019, 04/30/2019 07/18/2019, 11/30/2019	N/A

## 4.16 Oakland West

Station Information for Oakland West	
AQS ID	06-001-0011
GPS coordinates	37.814781, -122.282347
Location	Shelter in parking lot
Address	1100 21 <sup>st</sup> St, Oakland, CA 94607
County	Alameda
Distance to road from gaseous probe (meters)	Grand Ave: 34 Linden St: 33 Adeline St: 168 21 <sup>st</sup> St: 80
Traffic count (AADT, year)	Grand Ave: 19,796 (2012) Linden St: 500 (2015) Adeline St: 8,596 (2013) 21 <sup>st</sup> St: 600 (2015) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

The Air District opened a monitoring station one mile downwind of the Port of Oakland in February 2009 because the Port of Oakland is considered a major area source of diesel particulate matter emissions. Studies have shown that the West Oakland community is exposed to higher concentrations of diesel particulate matter than elsewhere in the Bay Area, resulting in higher potential cancer risks. This site is one of the 40 nationwide sites for community monitoring of NO<sub>2</sub> in areas with susceptible and vulnerable populations.

Carbon monoxide, NO/NO<sub>2</sub>, and PM<sub>2.5</sub> are measured to determine the impact of emissions from the Port of Oakland and its associated diesel-truck traffic, and vehicle traffic from nearby highways. SO<sub>2</sub> is measured to determine the impact of emissions from ship traffic. Black carbon (BC) is measured to better determine the composition and relationship between BC and PM<sub>2.5</sub>.

VOC toxic compounds are sampled at Oakland West on a 1:12 schedule, and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded 21 exceedances of the national 24-hour PM<sub>2.5</sub> standard and the national 70 ppb 8-hour ozone standard was



exceeded on one day. No exceedances of the national standards for NO<sub>2</sub>, SO<sub>2</sub>, or CO were measured during the past three years.

## Oakland West Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1	SO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary	N/A
Parameter code	44201	42101	42601 / 42602	42401
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i	TECO 43i
Method code	047	054	074	060
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Neighborhood	Middle	Neighborhood	Neighborhood
Monitor start date	12/13/2010	02/25/2009	02/25/2009	02/25/2009
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	6	6	6	6
Distance from supporting structure (meters)	> 1	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	40	40	40	40
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	12	12	13	12
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/02/2019 12/16/2019	05/02/2019 12/16/2019	05/02/2019 12/16/2019	05/02/2019 12/16/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A

## Oakland West Monitor Information

Pollutant, POC	PM2.5, 3	Speciated PM2.5, 5	BC, 1	Toxics, 3
Primary/QA Collocated/Other	Primary	Other	N/A	N/A
Parameter code	88101	88502 (pm mass) – many others see SASS section	84313	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Research	Research	Research
Site type(s)	Population Oriented, Highest Concentration	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SPM	SPM	SPM
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Met One FEM BAM 1020	Met One SASS	Teledyne API AE-633	Xontech 910A
Method code	170	810	894	210
FRM/FEM/ARM/other	FEM	N/A	N/A	N/A
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	Air District	N/A	Air District
Reporting Agency	Air District	N/A	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Neighborhood
Monitor start date	12/18/2012	02/12/2009	03/17/2009	03/02/2009
Current Sampling frequency	Continuous	1:6	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5	5	5	6
Distance from supporting structure (meters)	>2	>2	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	40	39	40	40
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	No	No	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	N/A	N/A	Glass	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	Y	N	N/A	N/A
Frequency of flow rate verification for PM samplers	Bi-weekly	Monthly	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/19/2019, 05/01/2019 07/25/2019, 11/06/2019	02/19/2019, 05/01/2019 07/25/2019, 11/06/2019	N/A	N/A

## 4.17 Palo Alto Airport

Station Information for Palo Alto Airport	
AQS ID	06-085-2010
GPS coordinates	37.457621, -122.112286
Location	The end of the runway in the aircraft run-up zone
Address	1925 Embarcadero Road, Palo Alto, CA 94303
County	Santa Clara
Groundcover	Paved
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

To better assess lead emissions and possible public exposure to lead in the ambient air near general aviation airports, the EPA selected 15 airports from across the nation (see 40 CFR 58 Appendix D 4.5(a)(iii)). Palo Alto Airport was one of the 15 airports chosen by EPA for required TSP-lead monitoring due to expected lead emissions from piston engine aircraft utilizing this airport.

For these required airport lead monitoring sites, if the rolling three-month average exceeds 50% of the 0.15  $\mu\text{g}/\text{m}^3$  NAAQS, then the site will continue to operate. If concentrations are consistently below 50% of the NAAQS, monitoring agencies may request a waiver for EPA approval to discontinue airport lead monitoring.

Lead monitoring at this site began on February 3, 2012, but was extended indefinitely because monitoring results showed that lead concentrations exceed 50% of the NAAQS in all but one of the rolling three-month quarters since monitoring began. Lead monitoring ended on December 19, 2014, because Santa Clara County sold the property to the City of Palo Alto. The sale triggered an FAA review of various operational plans and permits, revealing that the lead sampler location violated FAA regulations. The closure date in AQS is December 23, 2014 (the date of the last audit). The Air District continues to work EPA to identify a suitable alternative.

## Palo Alto Airport Monitor Information

Pollutant, POC	Lead (TSP), 3
Primary/QA Collocated/Other	Primary
Parameter code	14129
Basic monitoring objective(s)	NAAQS Comparison & Research
Site type(s)	Source Oriented
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	Tisch TE-HVPLUS-BL
Method code	191
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	RTI
Reporting Agency	Air District
Spatial scale	Micro
Monitor start date	02/03/2012
Current Sampling frequency	1:6
Sampling season	01/01 - 12/31
Probe height (meters)	2.0
Distance from supporting structure (meters)	N/A
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	>20
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No
Unrestricted airflow (degrees)	360
Probe material for reactive gases	N/A
Residence time for reactive gases (seconds)	N/A
Will there be changes within the next 18 months?	Yes – closed Dec 2014, working with EPA on alternative
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	Quarterly
Frequency of one-point QC check for gaseous instruments	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	Site closed Dec 2014 due to FAA violations in siting

## 4.18 Pittsburg

Station Information for Pittsburg	
AQS ID	Not applicable
GPS coordinates	38.007069, -121.868056
Location	Shelter
Address	1398 E Leland Rd, Pittsburg, CA, 94565
County	Contra Costa
Distance to road from gaseous probe (meters)	E Leland Rd: 75 Loveridge Rd: 260
Traffic count (AADT, year)	E Leland Rd: 25,080 (2006) Loveridge Rd: 23,432 (2006) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Vegetative
Statistical Area	San Francisco-Oakland-Hayward CBSA

This station is located in the urban area of Pittsburg (population 63,264). The station was established in June 2017 to provide additional black carbon and air toxics data in the community. Pittsburg is located along a transport corridor between the Bay Area and the Central Valley, and is in the vicinity/downwind of several industrial facilities along the Carquinez Strait.

This site is operated as part of the Air District's Toxics Program with samples taken on a 1:12 schedule. Samples are collected using a Xontech canister and are analyzed in the Air District laboratory. More information about the VOC toxics monitoring program can be found in the Toxics Program section of this report.

Data collected at this air monitoring station are available upon request and are not submitted to the EPA's AQS database.

## Pittsburg Monitor Information

Pollutant, POC	BC, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	N/A
Parameter code	84313	See toxics section
Basic monitoring objective(s)	Research	Research
Site type(s)	Population Oriented	Population Oriented
Monitor type(s)	SPM	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Teledyne API AE-633	Xontech 910
Method code	894	210
FRM/FEM/ARM/other	N/A	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Neighborhood
Monitor start date	06/27/2017	06/27/2017
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	3	3
Distance from supporting structure (meters)	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	None	None
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A

#### 4.19 Pleasanton (near-road)

Station Information for Laney College	
AQS ID	06-001-0015
GPS coordinates	37.701222, 121.903019
Location	Interstate 580 near Hopyard interchange
Address	Owen's Court, Pleasanton, CA
County	Alameda
Distance to road from gaseous probe (meters)	Owen's Court: 53 I-580: 179
Traffic count (AADT, year)	Owen's Court: 21,800 (2018) I-580: 231,500 (2016) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Gravel
Statistical Area	San Francisco-Oakland-Hayward CBSA

The Air District began monitoring pollutants at this site on April 1, 2018. The site was installed at the request of an Air District board member. The site is in Pleasanton in Alameda County, with a population of 70,285 according to the 2010 census.

This site monitors NO/NO<sub>2</sub>, CO, and PM<sub>2.5</sub>, and toxics. PM<sub>2.5</sub> monitoring at this site is considered representative of area-wide concentrations within this major metropolitan region.

Toxic compounds are determined from canister samples taken at Pleasanton on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

The site type for NO/NO<sub>2</sub>, CO, and PM<sub>2.5</sub> in AQS and in the accompanying tables is source oriented and population oriented. The site is located in a commercial area in Pleasanton.

Since monitoring began on April 1, 2018, this site recorded 13 exceedances of the national 24-hour PM<sub>2.5</sub> standard. There were no exceedances of the national standards for NO<sub>2</sub> or CO.



## Pleasanton Monitor Information

Pollutant, POC	NO2, 1	CO, 1	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A	Primary	N/A
Parameter code	42601 / 42602	42101	88101	See toxics section
Basic monitoring objective(s)	Public Information	Public Information	Public Information	Public Information
Site type(s)	Source Impact & Population Oriented	Source Impact & Population Oriented	Source Impact & Population Oriented	Population Oriented
Monitor type(s)	SPM	SPM	SPM	SPM
Network affiliation(s)	Near Road	Near Road	Near Road	N/A
Instrument manufacturer and model	TECO 42i	TECO 48i	Met One FEM BAM 1020	Xontech 901
Method code	074	054	170	210
FRM/FEM/ARM/other	FRM	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	Air District
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Micro	Micro	Micro	Urban
Monitor start date	04/01/2018	04/01/2018	04/01/2018	04/01/2018
Current Sampling frequency	Continuous	Continuous	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	5	5	5	5
Distance from supporting structure (meters)	>1	>1	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	None	None	None	None
Distance to furnace or incinerator flue (meters)	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	N/A	Glass
Residence time for reactive gases (seconds)	14	14	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	N/A	N/A
Dates of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/29/2019 08/08/2019	01/29/2019 08/08/2019	N/A	N/A
Date of semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	01/29/2019 05/31/2019 08/08/2019 11/04/2019	N/A

## 4.20 Point Richmond

Station Information for Point Richmond	
AQS ID	06-013-0005
GPS coordinates	37.926162, -122.385561
Location	Air monitoring shelter next to fire station
Address	140 W. Richmond Ave, Richmond, CA 94801
County	Contra Costa
Distance to road From gaseous probe (meters)	Washington Ave: 25 W. Richmond Ave: 10 Park Place: 27 Interstate 580: 266
Traffic count (AADT, year)	Washington Ave: 1,587 (2017) W. Richmond Ave: 4,405 (2006) Park Place: 1,877 (2017) Interstate 580: 82,000 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Point Richmond was chosen for H<sub>2</sub>S source-oriented monitoring because the community is near the southern fence line of the Chevron refinery. The monitoring site is located in downtown Point Richmond, 0.2 miles south of the Chevron refinery boundary. Point Richmond, a neighborhood within the city of Richmond, has a population of 3,780 according to the 2010 census.

Although prevailing winds in the area are from the south-southwest, occasional northerly winds will transport H<sub>2</sub>S emissions from the refinery over the community. H<sub>2</sub>S gases at Chevron can be emitted from the processing units, one mile to the north, or the Chevron Richmond Long Wharf Complex, one mile to the west, where crude oil and other feedstock chemicals from tankers are unloaded.

## Point Richmond Monitor Information

Pollutant, POC	H2S, 1
Primary/QA Collocated/Other	N/A
Parameter code	42402
Basic monitoring objective(s)	Public Information
Site type(s)	Population Oriented& Source Impact
Monitor type(s)	SPM
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 43i
Method code	020
FRM/FEM/ARM/other	N/A
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Neighborhood
Monitor start date	01/01/1999
Current Sampling frequency	Continuous
Sampling season	01/01 - 12/31
Probe height (meters)	3
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from trees (meters)	17
Distance to furnace or incinerator flue (meters)	7
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	7
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Every other week
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/11/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

## 4.21 Redwood City

Station Information for Redwood City	
AQS ID	06-081-1001
GPS coordinates	37.482934, -122.203500
Location	One-story commercial building
Address	897 Barron Ave, Redwood City, CA 94063
County	San Mateo
Distance to road from gaseous probe (meters)	Barron Ave: 13 Bay Road: 24 Warrington Ave: 131 US Highway 101: 455
Traffic count (AADT, year)	Barron Ave: 1,100 (2020)    Warrington Ave: 1,400 (2020) Bay Road: 3,770 (2012)    U.S. Highway 101: 222,600 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Being midway between San Francisco and San Jose, the Redwood City site is well positioned to monitor ozone precursors and ozone moving southward across the peninsula as they are channeled by the coastal mountains to the west. Generally, Redwood City characterizes an area between South San Francisco and Palo Alto, which has a low air pollution potential due to the frequent presence of the sea breeze. Although the sea breeze typically keeps pollution levels low, when winds are light, high levels of ozone precursors, ozone, or particulates can occur due to the large number of sources in the area.

The air monitoring site is located in a commercial/industrial zone bordered by U.S. Highway 101 on one side and residential areas on the other three sides. NO/NO<sub>2</sub> and ozone are monitored because the area is a large source of ozone precursor emissions and ozone. Carbon monoxide is monitored because of the high traffic volume in the area with U.S. Highway 101, 0.3 miles north of the site. PM<sub>2.5</sub> is monitored because light winds combined with surface-based inversions during the winter months can cause particulate levels to become elevated.

VOC toxic compounds are sampled at Redwood City on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded four exceedances of the national 70 ppb 8-hour ozone standard and 19 exceedances of the national 24-hr PM<sub>2.5</sub>

standard. No exceedances of the national standards for NO<sub>2</sub> or CO were measured during the last three years.

## Redwood City Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	07/01/1976	03/01/1967	03/01/1967
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	7	7	7
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	46	46	46
Distance to furnace or incinerator flue (meters)	13	13	13
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	15	16	16
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/07/2019 08/21/2019	03/07/2019 08/21/2019	03/07/2019 08/21/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## Redwood City Monitor Information

Pollutant, POC	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A
Parameter code	88101	See Toxics Section
Basic monitoring objective(s)	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Met One FEM BAM 1020	Xontech 901
Method code	170	210
FRM/FEM/ARM/other	FEM	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Neighborhood
Monitor start date	10/01/2009	7/11/2001
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 - 12/31	01/01 - 12 /31
Probe height (meters)	6	7
Distance from supporting structure (meters)	>2	>2
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	40	10
Distance to furnace or incinerator flue (meters)	14	13
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	Y	N/A
Frequency of flow rate verification for PM samplers	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/07/2019, 05/13/2019 08/20/2019, 11/18/2019	N/A

## 4.22 Reid-Hillview Airport

Station Information for Reid-Hillview Airport	
AQS ID	06-085-2011
GPS coordinates	37.329841, -121.815438
Location	The end of the runway in the aircraft run-up zone
Address	2500 Cunningham Ave., San Jose, CA 95148
County	Santa Clara
Groundcover	Paved
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

To better assess lead emissions and possible public exposure to lead in the ambient air near general aviation airports, the EPA selected 15 airports from across the nation (see 40 CFR 58 Appendix D 4.5(a)(iii)).

Reid-Hillview Airport was one of the 15 airports chosen by EPA for required TSP-lead monitoring due to expected lead emissions from piston engine aircraft utilizing this airport.

For these required airport lead monitoring sites, if the rolling three-month average exceeds 50% of the  $0.15 \mu\text{g}/\text{m}^3$  NAAQS, then the site will continue to operate. If concentrations are consistently below 50% of the NAAQS, monitoring agencies may request a waiver for EPA approval to discontinue airport lead monitoring. For Reid-Hillview airport, results through December 2019 indicate that lead concentrations exceeded 50% of the NAAQS in one of the rolling three-month quarters. Three-month rolling averages from 2017 through 2019 at this site ranged from  $0.031 \mu\text{g}/\text{m}^3$  to  $0.085 \mu\text{g}/\text{m}^3$ .

## Reid-Hillview Airport Monitor Information

Pollutant, POC	Lead (TSP), 3
Primary/QA Collocated/Other	Primary
Parameter code	14129
Basic monitoring objective(s)	NAAQS Comparison & Research
Site type(s)	Source Oriented
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	Tisch TE-HVPLUS-BL
Method code	191
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	ERG
Reporting Agency	Air District
Spatial scale	Micro
Monitor start date	02/03/2012
Current Sampling frequency	1:6
Sampling season	01/01 - 12/31
Probe height (meters)	1.6 <sup>a</sup>
Distance from supporting structure (meters)	N/A
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	> 20
Distance to furnace or incinerator flue (meters)	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No
Unrestricted airflow (degrees)	360
Probe material for reactive gases	N/A
Residence time for reactive gases (seconds)	N/A
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	Quarterly
Frequency of one-point QC check for gaseous instruments	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/26/2019, 06/24/2019 09/25/2019, 12/19/2019

- a The probe height of the lead sampler at Reid-Hillview is set to the height of the fence standing between the samplers and Tully Road in order to place the sampler within the area designated by EPA for sampling. This was a requirement of the Reid-Hillview Airport and was designed to ensure that the samplers were in unquestionable compliance with the FAA requirements in 14 CFR Part 77. Operation of the samplers at the airport was contingent on meeting this requirement. Movement of the sampler to achieve a probe height greater than or equal to 2 meters would result in the sampler being located off airport property.



## 4.23 Richmond 7<sup>th</sup>

Station Information for Richmond 7 <sup>th</sup>	
AQS ID	06-013-0006
GPS coordinates	37.948172, -122.364852
Location	Fire station
Address	1065 7 <sup>th</sup> Street, Richmond, CA 94801
County	Contra Costa
Distance to road from gaseous probe (meters)	7 <sup>th</sup> St: 22 Hensley St: 30 Richmond Parkway: 200
Traffic count (AADT, year)	7 <sup>th</sup> St: 3,546 (2012) Hensley St: 3,700 (2012) Richmond Parkway: 32,000 (2012) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Richmond 7<sup>th</sup> Street was chosen for H<sub>2</sub>S and SO<sub>2</sub> source-oriented monitoring because it is near the eastern fence line of the Chevron refinery. Richmond has a population of 103,701 per the 2010 census and the site is located 0.5 miles east of the refinery boundary where public exposure to the highest H<sub>2</sub>S and SO<sub>2</sub> concentrations are expected. Normally, monitoring is done downwind of the prevailing wind direction. However, the prevailing winds are from the south, and carry emissions over San Pablo Bay. Because it is impractical to monitor over San Pablo Bay, a monitoring site was chosen downwind of the secondary wind direction, on the east side of the refinery.

VOC toxic compounds are sampled at Richmond 7<sup>th</sup> on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

SO<sub>2</sub> concentrations measured at Richmond 7<sup>th</sup> did not exceed the national 1-hour 75 ppb standard during the last three years.

## Richmond 7<sup>th</sup> Monitor Information

Pollutant, POC	SO2, 1	H2S, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	N/A	N/A
Parameter code	42401	42402	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Public information	Research
Site type(s)	Population Oriented & Source Impact	Population Oriented & Source Impact	Population Oriented
Monitor type(s)	SLAMS	SPM	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 43i	TECO 43i	Xontech 901
Method code	060	020	210
FRM/FEM/ARM/other	FEM	N/A	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	07/01/1980	01/01/1999	10/14/1992
Current Sampling frequency	Continuous	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	8	8	8
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	10	10	10
Distance to furnace or incinerator flue (meters)	12	12	12
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Glass
Residence time for reactive gases (seconds)	8	9	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other week	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/10/2019	04/10/2019	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

#### 4.24 Rodeo

Station Information for Rodeo	
AQS ID	06-013-0007
GPS coordinates	38.034331, -122.270336
Location	Single story storage area at fire station
Address	326 Third Street, Rodeo, CA 94572
County	Contra Costa
Distance to road from gaseous probe (meters)	Third St: 13 Parker St: 249
Traffic count (AADT, year)	Third St: 500 (2007) Parker St: 9,484 (2013) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

Rodeo was chosen for H<sub>2</sub>S source-oriented monitoring because the Phillips 66 refinery is on the northeastern boundary of the city (population 8,679 per the 2010 census). The monitoring site is in a residential area 0.6 miles southwest of the refinery. Although the prevailing winds in the area are from the southwest, northeast winds can transport H<sub>2</sub>S emissions from the refinery over the populated area of the town.

## Rodeo Monitor Information

Pollutant, POC	H2S, 1
Primary/QA Collocated/Other	N/A
Parameter code	42402
Basic monitoring objective(s)	Public information
Site type(s)	Population Oriented & Source Impact
Monitor type(s)	SPM
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 43i
Method code	020
FRM/FEM/ARM/other	N/A
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Neighborhood
Monitor start date	04/01/2002
Current Sampling frequency	Continuous
Sampling season	01/01 – 12/31
Probe height (meters)	7
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None
Distance from trees (meters)	> 50
Distance to furnace or incinerator flue (meters)	11
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	6
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Every other week
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/10/2019 07/01/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

## 4.25 San Carlos Airport (II)

Station Information for San Carlos Airport (II)	
AQS ID	06-081-2004
GPS coordinates	37.508162, -122.246305
Location	The end of the runway in the aircraft run-up zone
Address	620 Airport Drive, San Carlos, CA 94070
County	San Mateo
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

To better assess lead emissions and possible public exposure to lead in the ambient air near general aviation airports, the EPA selected 15 airports from across the nation (see 40 CFR 58 Appendix D 4.5(a)(iii)). San Carlos Airport was one of the 15 airports chosen by EPA for required TSP-lead monitoring due to expected lead emissions from piston engine aircraft utilizing this airport.

For these required airport lead monitoring sites, if the rolling three-month average exceeds 50% of the 0.15  $\mu\text{g}/\text{m}^3$  NAAQS, then the site will continue to operate. If concentrations are consistently below 50% of the NAAQS, monitoring agencies may request a waiver for EPA approval to discontinue airport lead monitoring.

Lead monitoring at the San Carlos II site (both primary and collocated) started on March 25, 2015. The original San Carlos Airport I site was inappropriately sited and had to be moved because it violated FAA air space restrictions. This new site has a different AQS site ID (06-081-2004) than the original San Carlos Airport I site because the new site is about 120 meters to the southeast and farther away from the aircraft run-up area. Three-month rolling averages during 2015 and 2016 at this site ranged from 0.016  $\mu\text{g}/\text{m}^3$  to 0.025  $\mu\text{g}/\text{m}^3$ .

As of Tuesday, April 11, 2017, the TSP-Pb monitoring at the San Carlos Airport II monitoring site has been discontinued due to circumstances beyond the Air District's control. The Air District notified EPA of the discontinuation of data collection on April 13, 2017. See Sections 2.2.9 and 2.4 for more details.

The Air District will continue to work with EPA to find a suitable alternative.

## San Carlos Airport (II) Monitor Information

Pollutant, POC	Lead (TSP), 3	Lead (TSP), 5
Primary/QA Collocated/Other	Primary	QA Collocated
Parameter code	14129	14129
Basic monitoring objective(s)	NAAQS Comparison & Research	NAAQS Comparison & Research
Site type(s)	Source Oriented	Source Oriented
Monitor type(s)	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Tisch TE-HVPLUS-BL	Tisch TE-HVPLUS-BL
Method code	191	191
FRM/FEM/ARM/other	FEM	FEM
Collecting Agency	Air District	Air District
Analytical Lab	ERG	ERG
Reporting Agency	Air District	Air District
Spatial scale	Micro	Micro
Monitor start date	03/25/2015	03/25/2015
Current Sampling frequency	1:6	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	2.1	2.1
Distance from supporting structure (meters)	N/A	N/A
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	>30	>30
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	2.8	2.8
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	No
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	N/A
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	No	No
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Quarterly
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Dates of semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A

## 4.26 San Francisco

Station Information for San Francisco		
AQS ID	06-075-0005	
GPS coordinates	37.765946, -122.399044	
Location	One-story commercial building	
Address	10 Arkansas St, Suite N, San Francisco, CA 94107	
County	San Francisco	
Distance to road from gaseous probe (meters)	16 <sup>th</sup> St: 32 Arkansas St: 17	Interstate 280: 300 U.S. Highway 101: 504
Traffic count (AADT, year)	16 <sup>th</sup> St: 11,764 (2012) Arkansas St: 1,750 (2015) Interstate 280: 106,000 (2015) U.S. Highway 101: 226,000 (2015) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.	
Groundcover	Paved	
Statistical Area	San Francisco-Oakland-Hayward CBSA	

Although the sea breeze usually keeps pollution levels low, light wind conditions can result in high levels of ozone precursors or particulates due to the large number of sources in San Francisco. The east side of the city was selected for air monitoring because it is densely populated (including many daytime visitors and commuters), has some industry, and, as a transportation hub, has generally higher traffic volume. The site is located near the fringe of the central business district, in an area of light industry that is close to a residential area and two major freeways.

Ozone and NO/NO<sub>2</sub> are measured to monitor population exposure to these pollutants, and because this is a source area for ozone precursors. Carbon monoxide is measured due to high traffic volume. PM<sub>10</sub> and PM<sub>2.5</sub> are measured due to stagnant days, surface-based inversions, and heavy vehicular traffic can cause elevated PM levels.

PM<sub>10</sub> monitoring was changed from 1:6 to 1:12 sampling effective January 1, 2013 to accommodate limited resources. Because the Bay Area is well above the minimum monitoring requirements for PM<sub>10</sub>, EPA approved this decrease in sampling frequency as well as converting these PM<sub>10</sub> monitors from SLAMS to SPMs. Therefore, this monitor is no longer counted in PM<sub>10</sub> minimum monitoring requirements.

VOC toxic compounds are sampled at San Francisco by both the Air District and CARB on a 1:12 schedule and analyzed by their respective laboratories. Carbonyls and metals are also sampled by CARB on the same 1:12 schedule. Details about the CARB toxics monitoring program can be found at <http://www.arb.ca.gov/toxics/toxics.htm>.

Information about toxics monitoring by the Air District can be found in the Toxics Program section of this report.

During the most recent three years, there were 21 exceedances of the 24-hour National PM<sub>2.5</sub> standard and no exceedances of the national standards for ozone, PM<sub>10</sub>, NO<sub>2</sub> or CO.



## San Francisco Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	01/01/1986	01/01/1986	NO: 12/01/1985 NO2: 01/01/1986
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	11	11	11
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	15	15	15
Distance to furnace or incinerator flue (meters)	5	5	5
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	13	13	14
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/21/2019 11/19/2019	05/21/2019 11/19/2019	05/21/2019 11/19/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## San Francisco Monitor Information

Pollutant, POC	PM10, 1	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	Primary	N/A
Parameter code	81102	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SPM	SLAMS	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	Andersen HiVol 1200	Met One FEM BAM 1020	Xontech 910A
Method code	063	170	210
FRM/FEM/ARM/other	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	N/A	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	11/16/1986	10/01/2009	01/22/1991
Current Sampling frequency	1:12	Continuous	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	8	8	8
Distance from supporting structure (meters)	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	18	16	14
Distance to furnace or incinerator flue (meters)	7	7	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/11/2019, 05/20/2019 08/28/2019, 11/18/2019	03/11/2019, 05/20/2019 08/28/2019, 11/18/2019	N/A

## 4.27 San Jose – Jackson

Station Information for San Jose – Jackson	
AQS ID	06-085-0005
GPS coordinates	37.348497, -121.894898
Location	Top floor of two-story commercial building
Address	158 E. Jackson St, San Jose, CA 95112
County	Santa Clara
Distance to road from gaseous probe (meters)	Jackson St: 15 4 <sup>th</sup> St: 35
Traffic count (AADT, year)	Jackson St: 5,992 (2007) 4 <sup>th</sup> St: 7,300 (2014) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

The San Jose air monitoring site is in the center of northern Santa Clara Valley, in a commercial and residential part of downtown San Jose. This area is encircled by major freeways with an international airport 1.5 miles to the northwest.

Ozone precursors emitted within the central San Francisco Bay Area are often carried into the San Jose area by the prevailing northwesterly winds. The northern half of the Santa Clara Valley is densely populated, and the associated activities of the residents also add significant pollutant emissions into the air. The air quality in this location is representative of a large part of the valley due to the diurnal up-valley and down-valley air flow, which mixes the pollutants throughout the valley.

NO/NO<sub>2</sub> and ozone are monitored because of the large amount of ozone precursor emissions near the area as well as from upwind areas. Carbon monoxide is measured because of the significant traffic volume in the area. PM<sub>10</sub> and PM<sub>2.5</sub> are monitored because light winds combined with surface-based inversions within the valley during winter months can cause elevated particulate levels.

The San Jose – Jackson station was approved by EPA as an NCore multi-pollutant monitoring station on October 30, 2009 and NCore air monitoring began on January 1, 2011. NCore sites must measure, at a minimum, PM<sub>2.5</sub> using both continuous and filter-based samplers, speciated PM<sub>2.5</sub>, PM<sub>10-2.5</sub>, O<sub>3</sub>, SO<sub>2</sub>, CO, NO/NO<sub>y</sub>, wind speed, wind direction, relative humidity, and ambient temperature. More information about the NCore program is included in Section 5.3. In March 2014, the Air District requested a waiver (see APPENDIX F) to discontinue NO<sub>y</sub> monitoring for the NCore program because

2011-2013 data showed an insignificant statistical difference between NO<sub>x</sub> and NO<sub>y</sub>. Similar findings are shown using the 2014-2015 data. The EPA approved this request (see APPENDIX F). As part of the approval and the new requirements for the PAMS, the Air District is planning to monitor NO<sub>y</sub> at Livermore in 2019.

Gaseous VOC toxic compounds, carbonyls, PAHs, and metals are sampled on a 1:6 schedule as part of the NATTS program through June 30, 2018. The Air District laboratory analyzes samples for VOCs and carbonyls, the EPA national contract laboratory, currently ERG, analyzes samples for PAH's and PM<sub>10</sub> metals. The Air District left the NATTS program on July 1, 2018. CARB also does sampling for VOC toxic compounds, carbonyls, and metals at San Jose but on a 1:12 schedule with the analysis done by the CARB laboratory. More information about CARB toxics monitoring can be found at: <https://www.arb.ca.gov/aaqm/toxics.htm>. Information about toxics monitoring by the Air District can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded six exceedances of the national 70 ppb 8-hour ozone standard, 21 exceedances of the national 24-hour PM<sub>2.5</sub> standard, and one exceedance of the national 24-hour PM<sub>10</sub> standard. No exceedances of the national standards for NO<sub>2</sub>, SO<sub>2</sub>, or CO were measured during the last three years.

## San Jose – Jackson Monitor Information

Pollutant, POC	O3, 1	CO <sup>a</sup> , 1	NO2, 1	SO2 <sup>a</sup> , 1
Primary/QA Collocated/Other Parameter code	N/A 44201	N/A 42101	Primary 42601 / 42602	N/A 42401
Basic monitoring objective(s)	NAAQS comparison & Research	NAAQS comparison & Research	NAAQS comparison & Research	NAAQS comparison & Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s)	NCore	NCore	N/A	NCore
Instrument manufacturer and model	TECO 49i	TECO 48iTLE	TECO 42i	TECO 43iTLE
Method code	047	554	074	560
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Neighborhood
Monitor start date	11/01/2002	11/01/2002	11/01/2002	02/10/2009
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	12	12	12	12
Distance from supporting structure (meters)	>1	>1	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	>50	>50	>50	>50
Distance to furnace or incinerator flue (meters)	5	5	5	5
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	13	15	14	15
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/29/2019 11/12/2019	03/13/2019 08/19/2019	05/29/2019 11/12/2019	03/13/2019 08/19/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A

a Trace level instruments required for CO and SO<sub>2</sub> at NCore sites.

## San Jose – Jackson Monitor Information

Pollutant, POC	NO <sub>y</sub> , 2	PM10, 1	Toxics, 3
Primary/QA Collocated/Other	N/A	Primary	N/A
Parameter code	42600	81102	See toxics section
Basic monitoring objective(s)	Research	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SPM
Network affiliation(s)	NCore	N/A	N/A
Instrument manufacturer and model	API 200 EU/NOy	Partisol 2025 without VSCC	Xontech 924 & 901
Method code	699	127	202 & 210
FRM/FEM/ARM/other	N/A	FRM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	Air District	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	01/13/2011	10/15/2002	10/04/2002
Current Sampling frequency	Continuous	1:6	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 – 12/31
Probe height (meters)	12	9	10
Distance from supporting structure (meters)	> 1	>2	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	>50	> 50	> 50
Distance to furnace or incinerator flue (meters)	3	3	5
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	N/A	Glass
Residence time for reactive gases (seconds)	7	N/A	N/A
Will there be changes within the next 18 months?	Y <sup>a</sup>	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	Monthly	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	03/26/2019, 05/28/2019 08/14/2019, 11/06/2019	N/A

- a The EPA approved the waiver to shut down NO<sub>y</sub> monitor as required by the NCore program (see APPENDIX F). Under this approval, the Air District is planning to measure NO<sub>y</sub> at as part of the new PAMS requirement at Livermore in 2019.

## San Jose – Jackson Monitor Information

Pollutant, POC	PM10-2.5 (PMcoarse), 1	PM2.5, 1 <sup>a</sup>	PM2.5, 3	Speciated PM2.5, 5
Primary/QA Collocated/Other	Primary	QA Collocated	Primary	Other
Parameter code	86101	88101	88101	88502 (pm mass) – many others see SASS section
Basic monitoring objective(s)	Research	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented & Highest Conc.	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s)	NCore	NCore	NCore	NCore, CSN STN
Instrument manufacturer and model	Partisol 2025 without VSCC	Partisol-Plus 2025 w/VSCC	Met One FEM BAM 1020	Met One SASS
Method code	176	145	170	810
FRM/FEM/ARM/other	FRM	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	Air District	Air District	N/A	RTI
Reporting Agency	Air District	Air District	Air District	RTI
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Neighborhood
Monitor start date	1/1/2011	10/05/2002	10/01/2012	10/05/2002
Current Sampling frequency	1:3 (NCore)	1:3 (NCore)	Continuous	1:3
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	9	9	10	9
Distance from supporting structure (meters)	>2	>2	>2	>2
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	>50	>50	>50	>50
Distance to furnace or incinerator flue (meters)	2	2	4	3
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	4.0	4.0	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	No	No	No
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	N/A	N/A	N/A	N/A
Residence time for reactive gases (seconds)	N/A	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y	Y	N
Frequency of flow rate verification for PM samplers	Monthly	Monthly	Bi-weekly	Monthly
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/26/2019, 05/28/2019 08/14/2019, 11/06/2019	03/26/2019, 05/28/2019 08/14/2019, 11/06/2019	03/11/2019, 05/28/2019 08/14/2019, 11/06/2019	03/26/2019, 05/28/2019 08/14/2019, 11/06/2019

a PM<sub>2.5</sub> POC 1 was the primary sampler from October 2002 through September 2012 and was changed to be the collocated sampler after October 1, 2012 when PM<sub>2.5</sub> POC 3 became operational as the primary monitor.

#### 4.28 San Jose – Knox (near-road)

Station Information for San Jose – Knox	
AQS ID	06-085-0006
GPS coordinates	37.338202, -121.849892
Location	Trailer within 50m of freeway
Address	1007 Knox Ave. San Jose, CA 95122
County	Santa Clara
Distance to road from gaseous probe (meters)	Hwy 101: 16 I-280/680: 262 Story Rd: 234 Knox Ave: 236
Traffic count (AADT, year)	Hwy 101: 283,500 (2017) I-280/680: 211,000 (2017) Story Rd: 20,571 (2016) Knox Ave: 2,500 (2019) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Gravel
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

The Air District is monitoring pollutants at this site because it has the fourth highest Fleet Equivalent AADT (FE-AADT) in Santa Clara County. Road segments with higher FE-AADT values in Santa Clara County did not meet EPA siting requirements for monitoring (either the roadway was elevated or was otherwise in an unsafe location).

This site is monitoring NO/NO<sub>2</sub>, CO, PM<sub>2.5</sub>, Ultrafine Particulate Matter (UFP), black carbon (BC) and toxics. Toxics sampling began on August 15, 2014. Monitoring for all other parameters began on September 1, 2014. The site is located with the city of San Jose, which is the largest city in the Bay Area with a population of 945,942 according to the 2010 census.

Toxic compounds are determined from canister samples taken at San Jose - Knox on a 1:12 schedule and later analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

PM<sub>2.5</sub> monitoring at this site is considered representative of area-wide concentrations within this major metropolitan region.

The site type for NO/NO<sub>2</sub>, CO, and PM<sub>2.5</sub> in AQS and in the accompanying tables is source oriented and population oriented based on the similarity in pollutant



concentration with other nearby measurements. The site is within 0.25 miles of residential and commercial areas in San Jose.

During the most recent three years, this site recorded 23 exceedances of the national 24-hour PM<sub>2.5</sub> standard. No exceedances of the national standards for NO<sub>2</sub> were measured during the last three years.

## San Jose – Knox Monitor Information

Pollutant, POC	NO2, 1	CO, 1	PM2.5, 3	BC, 1	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A	Primary	N/A	N/A
Parameter code	42601 / 42602	42101	88101	84313	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	Public Information	Research
Site type(s)	Source Impact & Population Oriented	Source Impact & Population Oriented	Source Impact & Population Oriented	Source Impact	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SPM	SPM
Network affiliation(s)	Near Road	Near Road	Near Road	N/A	N/A
Instrument manufacturer and model	TECO 42i	TECO 48i	Met One FEM BAM 1020	Teledyne API AE-633	Xontech 901
Method code	074	054	170	894	210
FRM/FEM/ARM/other	FRM	FRM	FEM	N/A	N/A
Collecting Agency	Air District	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A	Air District
Reporting Agency	Air District	Air District	Air District	Air District	Air District
Spatial scale	Micro	Micro	Micro	Micro	Neighborhood
Monitor start date	09/01/2014	09/01/2014	09/01/2014	09/01/2014	08/15/2014
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31	01/01-12/31	01/01 – 12/31
Probe height (meters)	6	6	5	6	5
Distance from supporting structure (meters)	> 1	> 1	> 2	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None	None
Distance from trees (meters)	8 <sup>1</sup>	8 <sup>1</sup>	8 <sup>1</sup>	8	8
Distance to furnace or incinerator flue (meters)	None	None	None	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	N/A	N/A	Glass
Residence time for reactive gases (seconds)	16	15	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	Y	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	Bi-weekly	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	N/A	N/A	N/A
Dates of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	05/14/2019 12/10/2019	05/14/2019 12/10/2019	N/A	N/A	N/A
Dates semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	02/21/2019 05/14/2019 08/14/2019 12/10/2019	N/A	N/A

<sup>1</sup> Due to siting logistics constraints and in an effort to meet the objective of characterizing near-road emissions in the best segment in this MSA, the San Jose – Knox site was chosen even though the distance to the closest tree is less than 10 meters. Region 9 EPA

was involved in the development of this site, were aware of the tree placement, and concurred on the siting choice, approving this site as meeting the requirements for near-road monitoring.

#### 4.29 San Martin

<b>Station Information for San Martin</b>	
AQS ID	06-085-2006
GPS coordinates	37.079379, -121.600031
Location	Air monitoring shelter next to maintenance shed
Address	13030 Murphy Ave, San Martin, CA 95046
County	Santa Clara
Distance to road from gaseous probe (meters)	Murphy Ave: 57 US Highway 101: 455 Monterey Rd: 561 San Martin Ave: 931
Traffic count (AADT, year)	Murphy Ave: 1,768 (2018) US Highway 101: 128,100 (2017) Monterey Rd: 15,054 (2018) San Martin Ave: 7,795 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Vegetative
Statistical Area	San Jose-Sunnyvale-Santa Clara CBSA

San Martin was chosen for monitoring ozone because earlier field measurements showed this area to have the highest ozone concentrations in the Santa Clara Valley. Prevailing winds transport ozone and ozone precursors down the valley from the densely populated San Jose area as well as the surrounding San Francisco Bay. Because ozone is formed by a chemical reaction between organic and nitrogen oxide gases in the presence of sunlight, the highest ozone concentrations are usually observed tens of miles downwind from the highest concentration of emission sources (freeways, power generating facilities, etc.) because the reactions involving the organic gases are relatively slow.

San Martin is in an agricultural area at the south end of the Santa Clara Valley approximately 24 miles southeast of downtown San Jose and is a Census Designated Place (CDP) with a population of 7,027 based on the 2010 census. The monitoring site is located at the South County Airport, in the center of the valley and about 0.3 miles west of U.S. Highway 101.

During the most recent three years, this site recorded six exceedances of the national 70 ppb 8-hour ozone standard.

## San Martin Monitor Information

Pollutant, POC	O3, 1
Primary/QA Collocated/Other	N/A
Parameter code	44201
Basic monitoring objective(s)	NAAQS comparison
Site type(s)	Highest Conc. & Population Oriented & Regional Transport
Monitor type(s)	SLAMS
Network affiliation(s)	N/A
Instrument manufacturer and model	TECO 49i
Method code	047
FRM/FEM/ARM/other	FEM
Collecting Agency	Air District
Analytical Lab	N/A
Reporting Agency	Air District
Spatial scale	Urban
Monitor start date	04/30/1994
Current Sampling frequency	Continuous
Sampling season	01/01-12/31
Probe height (meters)	5
Distance from supporting structure (meters)	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	N/A
Distance from trees (meters)	26
Distance to furnace or incinerator flue (meters)	N/A
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A
Unrestricted airflow (degrees)	360
Probe material for reactive gases	Teflon
Residence time for reactive gases (seconds)	16
Will there be changes within the next 18 months?	N
Is it suitable for comparison against the annual PM2.5?	N/A
Frequency of flow rate verification for PM samplers	N/A
Frequency of one-point QC check for gaseous instruments	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	01/24/2019 04/03/2019 07/10/2019 10/02/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A

### 4.30 San Pablo

Station Information for San Pablo	
AQS ID	06-013-1004
GPS coordinates	37.960400, -122.356811
Location	One story commercial building
Address	1865-D Rumrill Blvd, San Pablo, CA 94806
County	Contra Costa
Distance to road from gaseous probe (meters)	Rumrill Blvd: 16
Traffic count (AADT, year)	Rumrill Blvd; 15,433 (2013) Traffic counts data were updated on April 1, 2019 and reflect the latest available data.
Groundcover	Paved
Statistical Area	San Francisco-Oakland-Hayward CBSA

San Pablo, with a population of 29,139 according to the 2010 census, was chosen for air monitoring because the city is in the most populated portion of western Contra Costa County. San Pablo is almost surrounded by the city of Richmond with a population of 103,701. This area of the county has heavy industry, high traffic volume including two major freeways, and is close to the Chevron refinery. Ozone and NO/NO<sub>2</sub> are measured because the area is downwind of the central San Francisco Bay Area, which is a large source of ozone precursor emissions. Carbon monoxide is measured due to the high traffic volume in the area. SO<sub>2</sub> is measured because the site is 1.2 miles downwind of the Chevron refinery, which can be a significant source of SO<sub>2</sub> emissions. PM<sub>2.5</sub> and PM<sub>10</sub> are measured because stagnant days in the fall and winter can result in elevated particulate levels. On October 19, 2016, a collocated PM<sub>10</sub> monitor was added to the site for quality assurance purpose.

A PM<sub>2.5</sub> continuous FEM began operation on December 12, 2012. The monitor is classified as middle scale based on its distance from the roadway and nearby traffic volume. The Air District considers this monitor to be comparable to the NAAQS because the monitor is representative of area-wide PM<sub>2.5</sub> concentrations.

The monitoring scale for ozone is middle scale. Following an EPA Region 9 review of the distance between the gaseous probe and the roadway, and the corresponding traffic count, EPA Region 9 suggested this monitor be changed from SLAMS to SPM and the Air District agreed to the change. Consequently, this monitor cannot be used toward meeting the minimum monitoring requirements for ozone.

VOC toxic compounds are sampled at San Pablo on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years this site recorded 24 exceedances of the national 24-hour PM<sub>2.5</sub> standard, two national 8-hour ozone standard, and one exceedance of the national 24-hour PM<sub>10</sub> standard. No national exceedances of the national standards for NO<sub>2</sub>, SO<sub>2</sub>, or CO were measured during the past three years.

## San Pablo Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1	SO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary	N/A
Parameter code	44201	42101	42601 / 42602	42401
Basic monitoring objective(s)	Public Information	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented & Source Impact
Monitor type(s)	SPM	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i	TECO 43i
Method code	047	054	074	060
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Middle	Middle	Middle	Neighborhood
Monitor start date	09/13/2002	09/13/2002	09/13/2002	09/13/2002
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	9	9	9	9
Distance from supporting structure (meters)	> 1	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	> 50	> 50	> 50	> 50
Distance to furnace or incinerator flue (meters)	7	7	7	7
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	9	10	10	9
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/17/2019 10/16/2019	04/17/2019 10/16/2019	04/17/2019 10/16/2019	04/17/2019 10/16/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A



## San Pablo Monitor Information

Pollutant, POC	PM10, 1	PM10, 2	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	QA Collocated	Primary	N/A
Parameter code	81102	81102	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS	SPM
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Tisch Env. HiVol TE-60	Tisch Env. HiVol TE-6000	Met One FEM BAM 1020	Xontech 901
Method code	141	141	170	210
FRM/FEM/ARM/other	FRM	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	Air District	Air District	Air District	Air District
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Middle	Middle	Middle	Middle
Monitor start date	09/23/2002	10/19/2016	12/12/2012	09/05/2002
Current Sampling frequency	1:6	1:12	Continuous	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	5	5	6	8
Distance from supporting structure (meters)	>2	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	>50	>50	>50	>50
Distance to furnace or incinerator flue (meters)	8	5	6	6
Distance between monitors fulfilling a QA collocation requirement (meters)	3	3	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	No	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	N/A	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Quarterly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/04/2019 04/16/2019 07/12/2019 10/15/2019	02/04/2019 04/16/2019 07/12/2019 10/15/2019	02/04/2019 04/16/2019 07/12/2019 10/15/2019	N/A

### 4.31 San Rafael

Station Information for San Rafael		
AQS ID	06-041-0001	
GPS coordinates	37.972310, -122.520004	
Location	Second floor of two-story commercial building	
Address	534 4 <sup>th</sup> Street, San Rafael, CA 94901	
County	Marin	
Distance to road from gaseous probe (meters)	4 <sup>th</sup> St: 18 US Highway 101: 112	Irwin St: 48 3 <sup>rd</sup> St: 124
Traffic count (AADT, year)	4 <sup>th</sup> St: 8,830 (2017)      Irwin St: 19,859 (2017) US Highway 101: 156,500 (2017)      3 <sup>rd</sup> St: 28,142 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.	
Groundcover	Paved	
Statistical Area	San Francisco-Oakland-Hayward CBSA	

San Rafael was chosen for air monitoring because it is the largest city in Marin County with a population of 57,713 according to the 2010 census. The city's climate and air quality are representative of that found throughout the populous eastern side of the county. Afternoon sea breezes typically keep pollution levels low. However, when the sea breeze is absent, local sources can cause elevated pollution levels.

The monitoring site is located at a commercial building about a block east of U.S. Highway 101 and near major highway access ramps. It is 0.5 miles east of the downtown San Rafael business district. There is no industrial activity in the immediate area. O<sub>3</sub> and NO/NO<sub>2</sub> are measured to monitor general population exposure to these pollutants. Carbon monoxide and PM<sub>10</sub> are measured because the site is close to a major transportation corridor. PM<sub>2.5</sub> is measured because light winds combined with wood burning, vehicular traffic, and surfaced-based inversions during winter can cause elevated particulate concentrations.

VOC toxic compounds are sampled at San Rafael on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

The monitoring scale for ozone is middle scale. Following an EPA Region 9 review of the distance between the gaseous probe and the roadway, and the corresponding traffic count, EPA Region 9 suggested this monitor be changed from SLAMS to SPM and the Air District agreed to the change. Consequently, this monitor cannot be used toward meeting the minimum monitoring requirements for ozone.

The PM<sub>2.5</sub> continuous FEM that has operated since 2009 was classified as middle scale based on its distance from the roadway and nearby traffic volume. The Air District considers this monitor to be comparable to the NAAQS because the monitor is representative of area-wide PM<sub>2.5</sub> concentrations.

During the most recent three years this site recorded 21 exceedances of the national 24-hour PM<sub>2.5</sub> standard and one exceedance of the national 24-hour PM<sub>10</sub> standard. No exceedances of the national standards for O<sub>3</sub>, NO<sub>2</sub>, or CO were recorded during the past three years.

## San Rafael Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	Public Information	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SPM	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Middle	Middle	Middle
Monitor start date	07/01/1976	10/01/1967	NO: 01/01/1968 NO2:10/01/1967
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	12	12	12
Distance from supporting structure (meters)	>1	>1	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	H Dist = 23 <sup>a</sup> V Dist above probe = 17	H Dist = 23 <sup>a</sup> V Dist above probe = 17	H Dist = 23 <sup>a</sup> V Dist above probe = 17
Distance from trees (meters)	14	14	14
Distance to furnace or incinerator flue (meters)	4	4	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	320	320	320
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	10	11	13
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	03/19/2019 08/27/2019	03/19/2019 08/27/2019	03/19/2019 08/27/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

- a The "obstruction not on the roof" is between zero degrees (north) and 40 degrees (northeast) leaving greater than 270 degrees of unobstructed airflow. The prevailing winds are from the south and lay within the unobstructed arc.

## San Rafael Monitor Information

Pollutant, POC	PM10, 1	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	Primary	N/A
Parameter code	81102	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SPM
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	Andersen HiVol 1200	Met One FEM BAM 1020	Xontech 901
Method code	063	170	210
FRM/FEM/ARM/other	FRM	FEM	N/A
Collecting Agency	Air District	Air District	Air District
Analytical Lab	Air District	N/A	Air District
Reporting Agency	Air District	Air District	Air District
Spatial scale	Middle	Middle	Middle
Monitor start date	11/04/1986	10/27/2009	01/01/1985
Current Sampling frequency	1:6	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	8	9	12
Distance from supporting structure (meters)	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	H Dist = 22 <sup>a</sup> V Dist above probe = 21	H Dist = 25 <sup>a</sup> V Dist above probe = 20	None
Distance from trees (meters)	13	10	14
Distance to furnace or incinerator flue (meters)	2	3	5
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	No	N/A	N/A
Unrestricted airflow (degrees)	320	320	360
Probe material for reactive gases	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	Y	N/A
Frequency of flow rate verification for PM samplers	Quarterly	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	03/18/2019, 06/17/2019 08/26/2019, 11/20/2019	03/19/2019, 06/17/2019 08/20/2019, 11/20/2019	N/A

- a The “obstruction not on the roof” is between zero degrees (north) and 40 degrees (northeast) leaving greater than 270 degrees of unobstructed airflow. The prevailing winds are from the south and lay within the unobstructed arc.

## 4.32 San Ramon

Station Information for San Ramon	
AQS ID	06-013-2007
GPS coordinates	37.743649, -121.934188
Location	Top of trailer
Address	9885 Alcosta Blvd, San Ramon, CA 94582
County	Contra Costa
Distance to road from gaseous probe (meters)	Alcosta Blvd (Montevideo): 300 Alcosta Blvd (S of Bollinger): 100 Pine Valley Rd: 350 Estero Dr: 250
Traffic count (AADT, year)	Alcosta Blvd (Montevideo): 9582 (2015) Alcosta Blvd (S. of Bollinger): 21,000 (2017) Pine Valley Rd: 9,500 (2018) Estero Dr: <500 (est. 2012) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Gravel
Statistical Area	San Francisco-Oakland-Hayward CBSA

San Ramon is also a population-oriented monitoring site, as the city has a population of 72,148 according to the 2010 census. The site is located along the I-680 corridor, which connects the Livermore Valley with the San Ramon Valley and other major cities of Contra Costa County.

During summer, localized north winds can be channeled southward from Concord and Walnut Creek along the I-680 corridor and pass through San Ramon before turning eastward into the Livermore Valley. Consequently, ozone and NO/NO<sub>2</sub> are measured at San Ramon in support of the Bay Area Photochemical Assessment Monitoring Stations (PAMS) program. Additionally, hourly speciated hydrocarbons are measured using a gas chromatograph analyzer for the PAMS program. A full description of the PAMS program can be found in the PAMS section of this document. In late 2013, the Air District decided to not operate the NO<sub>x</sub> monitor during winter.

The Air District chooses to operate all monitors at this site as PAMS-like sites that meet both Appendix E and Appendix A as allowed under Part 58.11(d). In operation for more than 24 months, these monitors are eligible for NAAQS comparison, but will continue as SPMs and not contribute to minimum monitoring design requirements.

During the most recent three years, this site recorded five exceedances of the national 70 ppb 8-hour ozone standard. During the same period, no exceedances of the national NO<sub>2</sub> standard have been measured.

### San Ramon Monitor Information

Pollutant, POC	O3, 1	NO2, 1
Primary/QA Collocated/Other	N/A	Primary
Parameter code	44201	42601 / 42602
Basic monitoring objective(s)	Research, NAAQS comparison	Research
Site type(s)	Population Oriented	Population Oriented
Monitor type(s)	SPM	SPM
Network affiliation(s)	Unofficial PAMS	Unofficial PAMS
Instrument manufacturer and model	TECO 49i	TECO 42i
Method code	047	074
FRM/FEM/ARM/other	FEM	FRM
Collecting Agency	Air District	Air District
Analytical Lab	N/A	N/A
Reporting Agency	Air District	Air District
Spatial scale	Urban	Urban
Monitor start date	01/01/2012	01/01/2012
Current Sampling frequency	Continuous	Continuous
Sampling season	04/01 – 11/30	01/01-11/30 in 2013 04/01-11/30 since 2014
Probe height (meters)	6	6
Distance from supporting structure (meters)	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	62	62
Distance to furnace or incinerator flue (meters)	None	None
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	Teflon	Teflon
Residence time for reactive gases (seconds)	18	18
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	06/13/2019 12/17/2019	06/13/2019 12/17/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A

### 4.33 Sebastopol

Station Information for Sebastopol	
AQS ID	06-097-0004
GPS coordinates	38.403765, -122.818294
Location	Top of two-story commercial building
Address	103 Morris Street, Sebastopol, CA 95472
County	Sonoma
Distance to road from gaseous probe (meters)	Morris St.: 80 Highway 12: 70
Traffic count (AADT, year)	Morris St.: 1,120 (2018) Highway 12: 23,000 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	Santa Rosa CBSA

Sebastopol's population was 7,379 according to the 2010 census. The city's climate is strongly influenced by the Pacific Ocean and the marine air flow is expected to keep pollution levels low.

There are no industrial sources in the immediate area. Ozone and NO/NO<sub>2</sub> are measured to monitor general population exposure to these pollutants. Carbon monoxide is measured because of the local urban traffic volume and proximity to the State Routes 12 and 116 corridors, which connect Sebastopol to surrounding rural portions of Sonoma County, a region known as West County, which has a population of up to 50,000 residents. PM<sub>2.5</sub> is measured because light winds combined with wood burning, vehicular traffic, and surface-based inversions in winter can cause elevated particulate concentrations.

VOC toxic compounds are sampled on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the past three years, this site recorded 17 national 24-hour PM<sub>2.5</sub> standard. No exceedances of the national standards for ozone, NO<sub>2</sub>, or CO in the past three years.



## Sebastopol Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary
Parameter code	44201	42101	42601 / 42602
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i
Method code	047	054	074
FRM/FEM/ARM/other	FEM	FRM	FRM
Collecting Agency	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood
Monitor start date	01/09/2014	01/09/2014	01/09/2014
Current Sampling frequency	Continuous	Continuous	Continuous
Sampling season	01/01 – 12/31	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	12	12	12
Distance from supporting structure (meters)	> 1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None
Distance from trees (meters)	12	12	12
Distance to furnace or incinerator flue (meters)	4	4	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	10	12	13
Will there be changes within the next 18 months?	N	N	N
Is it suitable for comparison against the annual PM2.5?	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	02/05/2019 07/17/2019	02/05/2019 07/17/2019	02/05/2019 07/17/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A

## Sebastopol Monitor Information

Pollutant, POC	PM2.5, 3	Toxics, 3
Primary/QA Collocated/Other	Primary	N/A
Parameter code	88101	See toxics section
Basic monitoring objective(s)	NAAQS comparison	Research
Site type(s)	Population Oriented & Highest Conc.	Population Oriented
Monitor type(s)	SLAMS	SPM
Network affiliation(s)	N/A	N/A
Instrument manufacturer and model	Met One FEM BAM 1020	Xontech 901
Method code	170	210
FRM/FEM/ARM/other	FEM	N/A
Collecting Agency	Air District	Air District
Analytical Lab	N/A	Air District
Reporting Agency	Air District	Air District
Spatial scale	Neighborhood	Neighborhood
Monitor start date	01/09/2014	01/11/2014
Current Sampling frequency	Continuous	1:12
Sampling season	01/01 – 12/31	01/01 – 12/31
Probe height (meters)	9	11
Distance from supporting structure (meters)	> 2	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None
Distance from trees (meters)	12	12
Distance to furnace or incinerator flue (meters)	4	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A
Unrestricted airflow (degrees)	360	360
Probe material for reactive gases	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A
Will there be changes within the next 18 months?	N	N
Is it suitable for comparison against the annual PM2.5?	Y	N/A
Frequency of flow rate verification for PM samplers	Bi-weekly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/04/2019, 04/22/2019 07/17/2019, 10/21/2019	N/A

#### 4.34 Vallejo

Station Information for Vallejo	
AQS ID	06-095-0004
GPS coordinates	38.102507, -122.237976
Location	One-story commercial building
Address	304 Tuolumne St, Vallejo, CA 94590
County	Solano
Distance to road from probe (meters)	Tuolumne St: 18      Solano Ave: 33 Capitol St: 30      Interstate 80: 700
Traffic count (AADT, year)	Tuolumne St: 8,332 (2008) Capitol St: 500 (2008) Solano Ave: 8,588 (2008) Interstate 80: 159,600 (2017) Traffic counts data were updated on April 1, 2020 and reflect the latest available data.
Groundcover	Paved
Statistical Area	Vallejo-Fairfield CBSA

The Vallejo monitoring site is located in a mixed commercial and residential neighborhood one mile east of downtown and 0.5 miles west of Interstate 80.

Ozone and NO/NO<sub>2</sub> are measured because southerly winds can transport ozone and its precursors into Vallejo from the heavily populated central Bay Area. Easterly winds can transport particulates from the Central Valley through the Carquinez Strait as data has shown this site to be impacted by transport of particulates into Vallejo during winter. Additionally, PM<sub>2.5</sub> can be elevated in Vallejo in winter due to local fireplace burning during nighttime temperature inversions when winds are light. from the Central Valley. Carbon monoxide is measured because Interstate 80 passes through the middle of the urban area east of the monitoring site. SO<sub>2</sub> is measured to monitor general population exposure and because refineries located to the south and east can be significant sources of SO<sub>2</sub>.

A collocated PM<sub>2.5</sub> FEM BAM is operated at Vallejo because this site has one of the highest PM<sub>2.5</sub> design values in the Bay Area.

VOC toxic compounds are sampled at Vallejo on a 1:12 schedule and analyzed in the Air District laboratory. More information about the toxics monitoring program can be found in the Toxics Program section of this report.

During the most recent three years, this site recorded three exceedances of the national 70 ppb 8-hour ozone standard, and 22 exceedances of the national 24-hour

PM<sub>2.5</sub> standard. No exceedances of the national standards for NO<sub>2</sub>, SO<sub>2</sub>, or CO were measured during the last three years.

### Vallejo Monitor Information

Pollutant, POC	O3, 1	CO, 1	NO2, 1	SO2, 1
Primary/QA Collocated/Other	N/A	N/A	Primary	N/A
Parameter code	44201	42101	42601 / 42602	42401
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	NAAQS comparison	NAAQS comparison
Site type(s)	Population Oriented	Population Oriented	Population Oriented	Population Oriented& Source Impact
Monitor type(s)	SLAMS	SLAMS	SLAMS	SLAMS
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	TECO 49i	TECO 48i	TECO 42i	TECO 43i
Method code	047	054	074	060
FRM/FEM/ARM/other	FEM	FRM	FRM	FEM
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	N/A	N/A	N/A	N/A
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Urban
Monitor start date	07/01/1976	07/01/1976	07/01/1976	07/01/1976
Current Sampling frequency	Continuous	Continuous	Continuous	Continuous
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31
Probe height (meters)	9	9	9	9
Distance from supporting structure (meters)	> 1	>1	> 1	> 1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	> 50	>50	> 50	>50
Distance to furnace or incinerator flue (meters)	4	4	4	4
Distance between monitors fulfilling a QA collocation requirement (meters)	N/A	N/A	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instruments(s).	N/A	N/A	N/A	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	Teflon	Teflon	Teflon	Teflon
Residence time for reactive gases (seconds)	8	10	10	10
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM <sub>2.5</sub> ?	N/A	N/A	N/A	N/A
Frequency of flow rate verification for PM samplers	N/A	N/A	N/A	N/A
Frequency of one-point QC check for gaseous instruments	Every other day	Every other day	Every other day	Every other day
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	04/24/2019 10/23/2019	04/24/2019 10/23/2019	04/24/2019 10/23/2019	04/24/2019 10/23/2019
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	N/A	N/A	N/A	N/A

## Vallejo Monitor Information

Pollutant, POC	PM2.5, 3	PM2.5, 4	PM2.5, 5 Speciated	Toxics, 3
Primary/QA Collocated/Other	Primary	QA Collocated	Other	N/A
Parameter code	88101	88101	88502 (pm mass) – many others see SASS section	See toxics section
Basic monitoring objective(s)	NAAQS comparison	NAAQS comparison	Research	Research
Site type(s)	Population Oriented & Highest Conc. & Regional Transport	Population Oriented	Population Oriented	Population Oriented
Monitor type(s)	SLAMS	SLAMS	SPM	SPM
Network affiliation(s)	N/A	N/A	N/A	N/A
Instrument manufacturer and model	Met One FEM BAM 1020	Met One FEM BAM 1020	Met One SASS	Xontech 901
Method code	170	170	810	210
FRM/FEM/ARM/other	FEM	FEM	N/A	N/A
Collecting Agency	Air District	Air District	Air District	Air District
Analytical Lab	Air District	Air District	Air District	Air District
Reporting Agency	Air District	Air District	Air District	Air District
Spatial scale	Neighborhood	Neighborhood	Neighborhood	Neighborhood
Monitor start date	01/01/2011	01/01/2013	06/11/2008	05/01/1986
Current Sampling frequency	Continuous	Continuous	1:6	1:12
Sampling season	01/01 - 12/31	01/01 - 12/31	01/01 - 12/31	01/01 – 12/31
Probe height (meters)	6	6	7	10
Distance from supporting structure (meters)	>2	>2	>2	>1
Distance from obstructions on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from obstructions not on roof (meters). Include horizontal distance + vertical height above probe for obstructions nearby (meters).	None	None	None	None
Distance from trees (meters)	>50	>50	>50	>50
Distance to furnace or incinerator flue (meters)	3	3	5	4
Distance between monitors fulfilling a QA collocation requirement (meters)	4	4	N/A	N/A
For low volume PM instruments (flow rate < 200 liters/minute) is any PM instrument within 1m of the LoVol? If yes, please list distance (meters) and instrument(s).	No	No	No	N/A
For high volume PM instrument (flow rate > 200 liters/minute), is any PM instrument within 2m of the HiVol? If yes, please list distance (meters) and instrument(s).	N/A	N/A	N/A	N/A
Unrestricted airflow (degrees)	360	360	360	360
Probe material for reactive gases	N/A	N/A	N/A	Glass
Residence time for reactive gases (seconds)	N/A	N/A	N/A	N/A
Will there be changes within the next 18 months?	N	N	N	N
Is it suitable for comparison against the annual PM2.5?	Y	Y	N	N/A
Frequency of flow rate verification for PM samplers	Bi-weekly	Bi-weekly	Monthly	N/A
Frequency of one-point QC check for gaseous instruments	N/A	N/A	N/A	N/A
Date of Annual Performance Evaluation conducted in the past calendar year for gaseous parameters (MM/DD/YYYY)	N/A	N/A	N/A	N/A
Date of two semi-annual flow rate audits conducted in the past calendar year for PM monitors (MM/DD/YYYY, MM/DD/YYYY)	02/06/2019 04/23/2019 07/29/2019 10/23/2019	02/06/2019 04/23/2019 07/29/2019 10/23/2019	02/06/2019 04/23/2019 07/29/2019 10/23/2019	N/A

## **5. SPECIAL MONITORING PROGRAMS CONDUCTED IN 2018**

## 5.1 Meteorology Program

The Air District operates a meteorological monitoring program to provide measurements of ambient meteorological parameters to meet the requirements of many programs within the Air District. Air District programs using meteorological data are: air quality forecasting, photochemical modeling, source modeling, and data analysis. To obtain high quality data to be used for regulatory applications, the Air District considers EPA recommendations for siting, instrumentation, data accuracy, and quality assurance.

The placement of meteorological stations depends on the use of the data. Sites chosen for air quality forecasting are located in areas that show the general wind and temperature patterns within the Air District. Photochemical modeling sites are chosen to show boundary conditions, general conditions, and upper air meteorological conditions. Source modeling sites are chosen to be representative of the source and receptor domain to be modeled. Sites used for data analysis are usually located near high pollution areas to determine the trajectories between source areas and downwind high concentration areas, as well as the general atmospheric conditions occurring during pollution episodes.

Because most Air District air monitoring stations are in urban or suburban neighborhoods where multistory buildings and trees are nearby, it is not possible to place meteorological systems at all Air District air monitoring stations that meet EPA meteorological siting recommendations. EPA recommends that wind systems be located at a height of 10 meters or at plume height if the use is source-oriented modeling. In addition, the distance between the wind instrument and any obstruction should be at least 10 times the height of the obstruction.

In 2019, the meteorological network consisted of 19 sites. Point San Pablo is currently being relocated due to vandalism cutting power to the station. Figure 5-1 shows their locations. Eight are adjacent to air monitoring stations (Bethel Island, Fairfield, Concord, San Ramon, Vallejo, Livermore, Gilroy, and San Martin). The other air monitoring stations have obstructions to air flow nearby, necessitating placement of the meteorological sites further away. Additionally, to meet forecasting or photochemical modeling needs, some meteorological sites have been placed on ridges or mountain-tops, such as at Chabot and Livermore. Sensors used in the Air District's meteorological network include wind speed and direction, temperature, relative humidity, precipitation, and pressure.

Hourly-averaged data are made available to Air District staff and the public on the Air District's web page and are archived in the Meteorology and Measurement

Division's database. Each site is visited monthly by Air District staff for a visual inspection of the instrumentation. A technician visits the site to correct problems. Data are also reviewed on an ongoing basis by Air District meteorologists producing daily air quality forecasts for the Bay Area.

Data recorded at airports, oil refineries, sewage treatment plants, universities, and private companies are included in the Meteorology and Measurement Division meteorological database if they meet EPA recommended siting and maintenance specifications. If requested by facilities, Air District staff will advise where to place meteorological stations and how to maintain the sensors to be used for regulatory purposes.





Figure 5-1. Map of Air District Meteorological Monitoring Sites in 2019

## **5.2 National Air Toxics Trends Station (NATTS) at San Jose**

EPA established the National Air Toxics Trends Stations (NATTS) network in 2003. The program was created to improve national toxics monitoring with the goal of identifying toxics trends in urban and rural settings in the United States. EPA and the Air District agreed to include San Jose Jackson in the NATTS network because San Jose is the largest city in Northern California with a 2010 population of 945,942 and the San Jose air monitoring station has long data record (since 1991). The Air District began operating a NATTS site at the San Jose Jackson air monitoring station on January 1, 2003, with samples taken on a 1:6 schedule through June 30, 2018. Starting July 1, 2018, air toxics monitoring at San Jose is no longer part of the NATTS program. Refer to 2018 Annual Network plan for additional information on Hazardous Air Pollutants (HAPs).

### 5.3 NCore Program

In October 2006 the EPA revised 40 CFR Parts 53 and 58 to enhance ambient air quality monitoring to improve air quality measurements. One significant revision was the requirement to establish National Core (NCore) multi-pollutant monitoring stations. These stations provide data on several pollutants at lower detection limits and replace the National Air Monitoring Station (NAMS) networks that previously existed. NCore stations are also used to monitor trends of pollutants already in attainment. EPA recognized that pollutants already in attainment, and likely to remain so, did not need to be measured at all sites in a monitoring network. NCore stations are located in areas that represent the highest pollution levels for both attainment and non-attainment pollutants within an agency's boundaries. By reducing the number of monitors needed in a network, agencies can allocate scarce resources to other monitoring programs.

NCore stations are intended to:

- Report data to the public in a timely manner through AirNow, air quality forecasting, and other public reporting mechanisms.
- Support development of emissions control strategies through air quality model evaluation and other observational methods.
- Track long-term trends for accountability of emissions control programs and health assessments that contribute to ongoing reviews and attainment of the National Ambient Air Quality Standards (NAAQS).
- Support scientific studies ranging across technological, health, and atmospheric disciplines including ecosystem assessments.

EPA designed the NCore network to have a mixture of urban and rural sites. In Northern California, EPA desired a monitoring station that would represent a large urban area. Recommendations for locating NCore urban sites are found in 40 CFR Part 58, Appendix D, and other EPA publications:

- Urban NCore stations are to be located at neighborhood or urban scale to provide representative exposure levels throughout the metropolitan area population.
- Urban NCore stations should be located where significant pollution levels exist.
- Population oriented monitoring is highly recommended.
- No biasing local pollutant emission sources should be within 500 meters at urban stations.

- Collocation with other network programs (such as NATTS, CSN, CASTNET, IMPROVE, NADP, PAMS) is encouraged.
- Siting of monitors at NCore sites must meet SLAMS requirements as specified in 40 CFR Part 58.

EPA and the Air District cooperatively agreed to establish the Northern California NCore station in San Jose effective January 1, 2011. San Jose was chosen as the NCore site because it is the city with largest population in the Bay Area with nearly one million residents based on 2010 census data. Exceedances of both the ozone and 24-hour PM<sub>2.5</sub> national standards have been measured in San Jose. Consequently, operating an NCore station in the San Jose area meets the requirement of being in an urban area with significant air pollution problems.

San Jose is located in the southern part of the Bay Area, and lies within the Santa Clara Valley. Wind patterns in the Santa Clara Valley are influenced greatly by the terrain, resulting in a prevailing flow roughly parallel to the valley's northwest-southeast orientation. During the daytime a sea breeze commonly carries pollutants from San Francisco, San Mateo, and Alameda counties southward into the Santa Clara Valley, while a drainage flow carrying pollutants toward the bay, in the opposite direction, occurs during the nighttime hours. This diurnal up valley and down valley air flow mixes pollutants throughout the valley, making San Jose representative of a large part of the Bay Area.

The monitoring objective for the current San Jose air quality monitoring station is population exposure. Monitoring at a population-oriented station is intended to represent air quality levels over a large area having a high population density. Consequently, the site cannot be too close to large emission sources such as industrial sources or highways, and the surrounding land use should be relatively uniform. EPA has defined neighborhood or urban scale as the appropriate area of representativeness for population-oriented monitoring. Neighborhood scale has dimensions of a 4-km radius around the monitoring station, and urban scale has a 50 km radius. Figure 5-2 shows the location of the current San Jose monitoring station, and a 4-km circle around the site representing a neighborhood scale area.

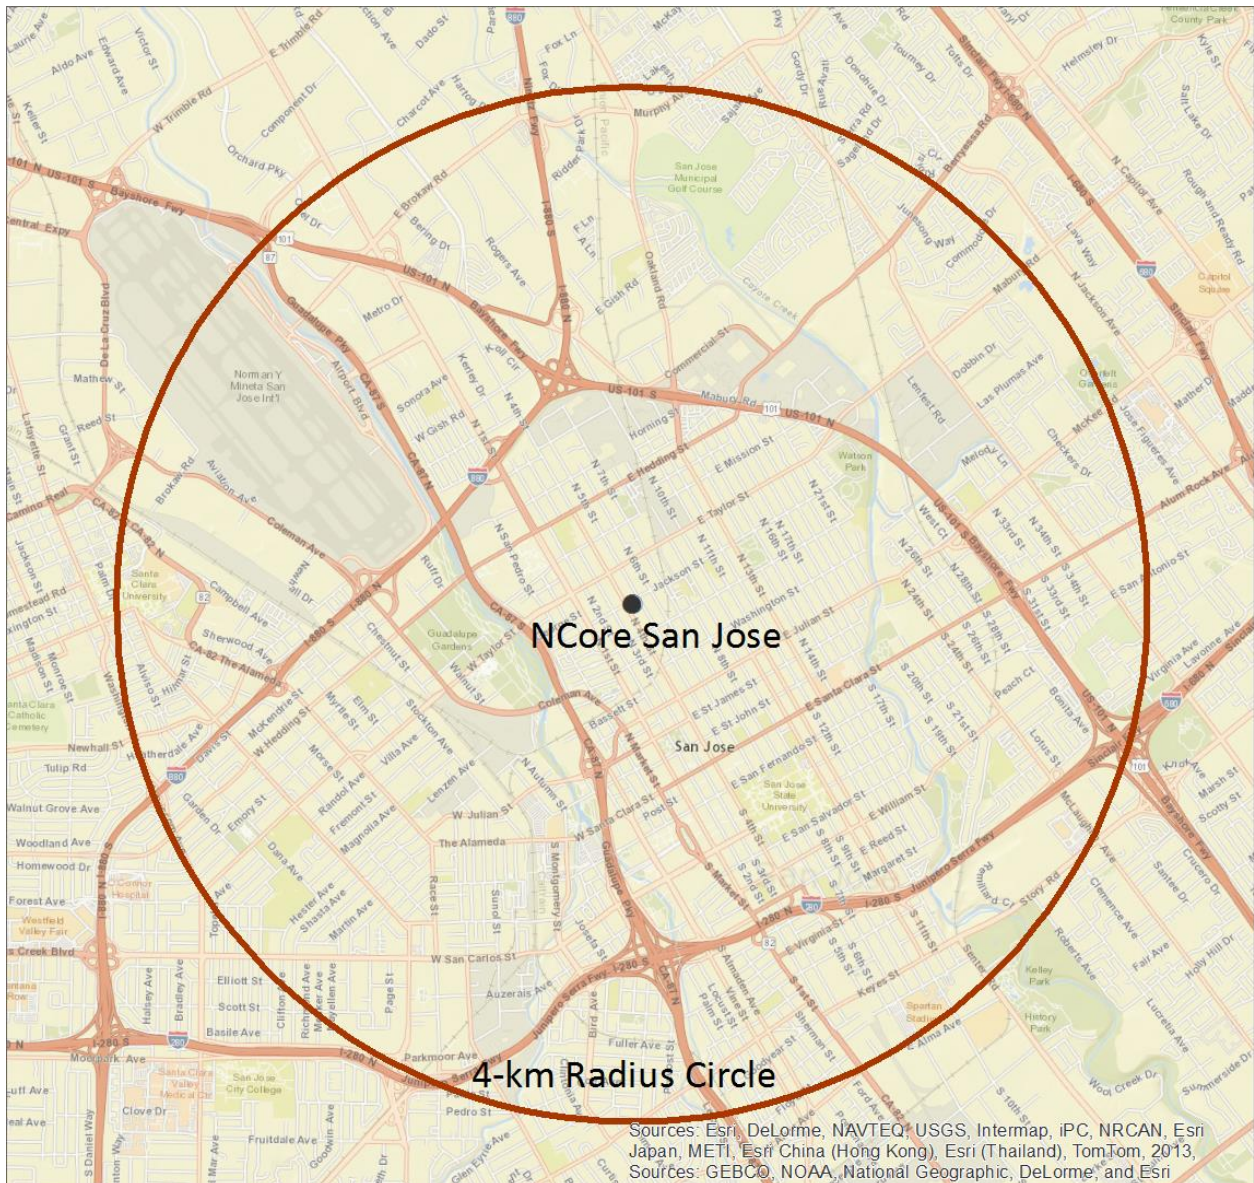


Figure 5-2. Map showing area of Neighborhood Scale at the San Jose NCore station

The map shows that the current station is in a residential/commercial area of San Jose. The station is located on Jackson Street, 1.6 km northwest of the downtown core. The Air District has operated air monitoring stations at various locations near downtown San Jose since 1968, and the current station has been in operation since 2002. The downtown area is encircled by freeways, but the closest freeway to the air monitoring station is 800 meters to the west-southwest, which is sufficiently distant to prevent vehicular emissions from dominating the general air quality at the San Jose station. San Jose International Airport is 2 to 4 km from the air monitoring station, distant enough that impacts from airport emissions would be relatively low at the monitoring station.

There are no large point sources within 500 meters of the station. The only significant emission sources within a 4-km radius of the San Jose air monitoring station are:

- The Norman Y. Mineta San Jose International Airport, located from 2-4 km NW of the site, is a significant source. The airport averaged 250 commercial and 81 general aviation departures and landings per day in 2015.
- Reed & Graham, Inc. (an asphalt batch plant), located 3.7 km SSW of the site.
- Central Concrete Supply Company, Inc., located 1.9 km SSW of the site.
- San Jose State University Cogeneration Plant, located 2.6 km SSE of the site.

The San Jose Jackson air monitoring station was located to provide air quality data representative of neighborhood scale monitoring. The station currently monitors all criteria pollutants, criteria pollutant precursors, and toxics. In addition to the NCore network, the site is part of the EPA STN network. Starting July 1, 2018, the San Jose Jackson air monitoring station is no longer part of NATTS program.

### **5.3.1 NCore Monitors**

Table 5-1 lists the NCore monitors operating at the San Jose Jackson station including the sampling methodology, sampling frequency, and spatial scale. Because ambient concentrations of the criteria pollutants CO and SO<sub>2</sub> are well below the NAAQS at population oriented sites across the U.S., EPA requires NCore sites to use higher sensitivity instruments than conventional instruments for these pollutants (note the use of Trace Level-Enhanced (TLE) type instruments for CO and SO<sub>2</sub>). PM<sub>10-2.5</sub> is measured using the difference between measurements of a pair of Partisol-Plus Model 2025 Sequential samplers, with one configured as a PM<sub>2.5</sub> sampler and the other configured as a PM<sub>10</sub> sampler.

On March 10, 2016, EPA issued a final rule revising monitoring requirements in 40 CFR Part 58. As a result, lead monitoring at NCore sites is not required after April 27, 2016.

In March 2014, the Air District requested a waiver to discontinue NO<sub>y</sub> monitoring at San Jose because the past three years of data showed an insignificant statistical difference between NO<sub>x</sub> and NO<sub>y</sub> (see APPENDIX E) and was approved by the EPA (see APPENDIX F). Under this approval, the District plans to monitor NO<sub>y</sub> at Livermore by July 31, 2019 and this site will become the official PAMS site in the Bay Area.

Table 5-1. NCore Monitors

<b>Monitor Type</b>	<b>Sampling Method</b>	<b>Sampling Frequency</b>	<b>Spatial Scale</b>
Carbon Monoxide (CO) trace level	TECO 48i TLE	Continuously	Neighborhood
Ozone (O <sub>3</sub> )	TECO 49i	Continuously	Neighborhood
Sulfur Dioxide (SO <sub>2</sub> ) trace level	TECO 43i TLE	Continuously	Neighborhood
PM <sub>2.5</sub> – filter-based FRM	Partisol-Plus 2025 w/VSCC	1:3	Neighborhood
PM <sub>2.5</sub> – continuous FEM	Met One FEM BAM 1020	Continuously	Neighborhood
PM <sub>2.5</sub> Speciation	Met One SASS	1:3	Neighborhood
Total Reactive Nitrogen (NO <sub>y</sub> )	API 200EU/NO <sub>y</sub>	Continuously	Neighborhood
Nitric Oxide (NO) from NO <sub>y</sub> monitor	API 200EU/NO <sub>y</sub>	Continuously	Neighborhood
PM <sub>10-2.5</sub>	Partisol-Plus 2025 Sequential PM <sub>10-2.5</sub> Air Sampler Pair	1:3	Neighborhood
Meteorological	EPA approved a waiver to use meteorological data from the San Jose Airport as official data for the NCore site.	Continuously	N.A.



## 5.4 Photochemical Assessment Monitoring Stations (PAMS)

This section describes the Air District's unofficial PAMS monitoring during 2019. For a discussion of upcoming changes to the Air District's PAMS monitoring to meet new EPA requirements under 40 CFR 58, Appendix D, Section 5(a), please see Appendix H.

Based on 40 CFR part 58, Appendix D, State air monitoring agencies are required to begin making PAMS measurements at their NCore location(s) by June 1, 2019. The EPA is delaying the start date for the revised Photochemical Assessment Monitoring Stations (PAMS) monitoring site network established in 40 CFR part 58, Appendix D. This final action extends the start date from June 1, 2019, to June 1, 2021. As a result of the delay the BAAQMD will not begin making PAMS measurements at the Livermore (approved NCore-waiver site location) in 2019, and will work with EPA to begin measurements on or before June 1, 2021.

The 1990 Clean Air Act Amendments required EPA to promulgate rules for the enhanced monitoring of ozone and its precursors (NO/NO<sub>2</sub> and VOCs) to collect information to address the continued nonattainment of the National Ambient Air Quality Standard (NAAQS) for ozone nationwide. Subsequent revisions to EPA's Air Monitoring regulations, 40 CFR Part 58, required air pollution agencies to establish Photochemical Assessment Monitoring Stations (PAMS) in ozone nonattainment areas classified as serious, severe, or extreme. The Bay Area is not in any of these categories but is in marginal nonattainment of the ozone NAAQS. However, the Air District chose to voluntarily conduct unofficial-PAMS monitoring to collect data that would improve our understanding of ozone formation in the area, which could be used to improve air quality forecasting and management activities. Monitoring began in 2010 (at Livermore) and in 2012 (at San Ramon).

The objectives of the Bay Area unofficial PAMS program are to:

- Measure air quality improvement progress by tracking ambient concentrations of ozone and ozone precursors.
- Improve photochemical model performance.
- Adjust ozone control strategies.

Traditionally, summertime Bay Area ozone concentrations are highest in the Livermore and Santa Clara Valleys. Meteorological conditions are ideal for ozone formation in these areas when precursor NO/NO<sub>2</sub> and VOCs are present in upwind areas. To better



understand the atmospheric chemistry, pollutant concentrations, emission reductions strategies, and transport, two locations in the Livermore area monitor for ozone and ozone precursors. Each PAMS site has meteorological wind and temperature sensors, as listed in Table 5-4.

Table 5-2. Monitoring start date for PAMS sites

Site	Parameter	Start Date for PAMS Data Collection
Livermore	Air Monitoring	August 1, 2010
	Meteorology	August 1, 2010
San Ramon	Air Monitoring	January 1, 2012 (NO/NO <sub>2</sub> )
		May 1, 2012 (VOC)
	Meteorology	December 14, 2011

The Air District’s long-existing Livermore air monitoring station was selected as a PAMS site because Livermore usually has the highest annual number of days exceeding the ozone NAAQS in the Bay Area. The site already had meteorological sensors measuring wind, temperature, and solar radiation; and air monitoring instruments measuring NO/NO<sub>2</sub> and ozone. Speciated VOCs were added to the San Ramon site in 2012. All ozone, NO/NO<sub>2</sub>, and VOC data are submitted to EPA’s AQ5 database.

The San Ramon site is a temporary site operated solely for the unofficial-PAMS program research. The San Ramon PAMS provides information on ozone precursors and ozone formation in the San Ramon Valley that may contribute to ozone concentrations in the Livermore Valley. The two PAMS locations are shown in Figure 5-3.

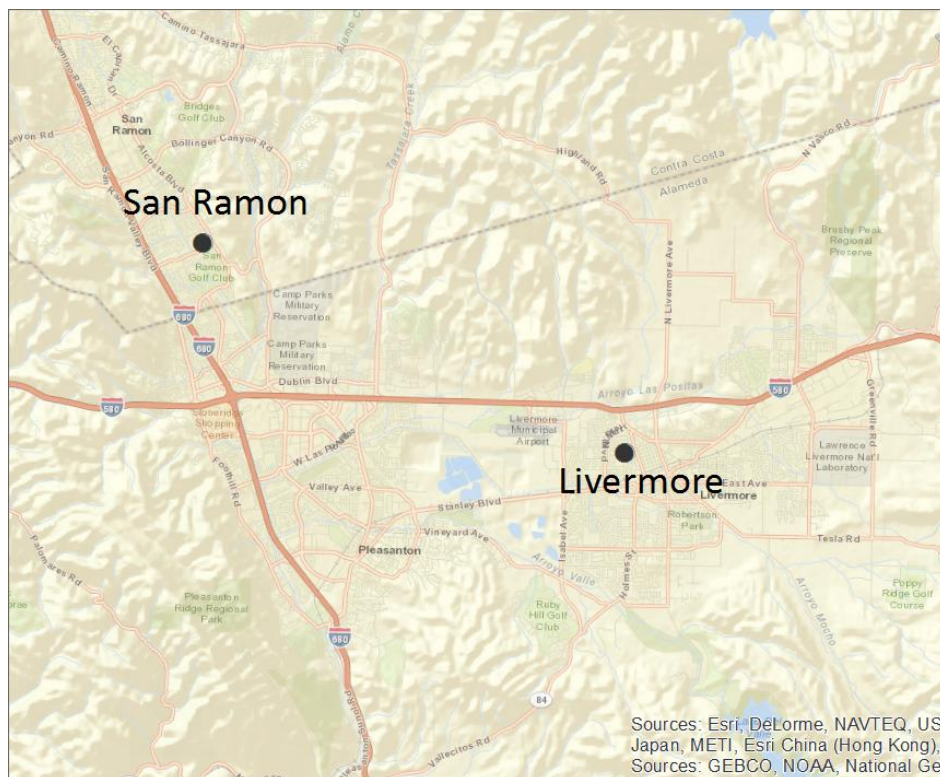


Figure 5-3. Map of the two PAMS sites in the Livermore Valley

Prior to November 2013, EPA identified 57 organic ozone precursor compounds usually measured at PAMS locations because of their significance in photochemical ozone pollution. On November 20, 2013, EPA released a memo (<http://www.epa.gov/ttn/amtic/files/ambient/pams/targetlist.pdf>) revising the photochemical assessment monitoring station compound target list. The revisions divide the previous list into two categories: priority compounds and optional compounds. In addition, seven new compounds were added to the priority list, for a total of 34 priority compounds and 29 optional compounds.

The Air District measures 56 compounds every hour using a gas chromatograph (GC) instrument. The GC does not analyze for two compounds EPA considers important ozone precursors: formaldehyde and acetone. The Air District determined that it is too costly to measure these compounds hourly. In addition, the GC does not measure the new priority compounds identified in the November 2013 EPA memo,  $\alpha/\beta$ -Pinene, 1,3 Butadiene, benzaldehyde, carbon tetrachloride, ethanol, and tetrachloroethylene. However, the GC does measure two additional compounds not on the EPA target list, 1-hexene and n-dodecane. Table 5-3 below lists the 56 compounds measured by the GC.

Table 5-3. List of speciated hydrocarbons measured by Gas Chromatograph in 2019

Compound	Parameter Code	Method Code
n-dodecane	43141	142
Ethane	43202	142
Ethylene	43203	142
Propane	43204	142
Propylene	43205	142
Acetylene	43206	142
n-butane	43212	142
Isobutane	43214	142
t-2-butene / trans-2-butene	43216	142
c-2-butene / cis-2-butene	43217	142
n-pentane	43220	142
Isopentane	43221	142
1-pentene	43224	142
t-2-pentene / trans-2-pentene	43226	142
c-2-pentene / cis-2-pentene	43227	142
3-methylpentane	43230	142

<b>Compound</b>	<b>Parameter Code</b>	<b>Method Code</b>
n-hexane	43231	142
n-heptane	43232	142
n-octane	43233	142
n-nonane	43235	142
n-decane	43238	142
Cyclopentane	43242	142
Isoprene	43243	142
2-2-dimethylbutane	43244	142
2-4-dimethylpentane	43247	142
1-hexene	43245	142
Cyclohexane	43248	142
3-methylhexane	43249	142
2-2-4-trimethylpentane	43250	142
2-3-4-trimethylpentane	43252	142
3-methylheptane	43253	142
Methylcyclohexane	43261	142
Methylcyclopentane	43262	142
2-methylhexane	43263	142
1-butene	43280	142
2-3-dimethylbutane	43284	142
2-methylpentane	43285	142
2-3-dimethylpentane	43291	142
n-undecane	43954	142
2-methylheptane	43960	142
m/p xylene	45109	142
Benzene	45201	142
Toluene	45202	142
Ethylbenzene	45203	142
o-xylene	45204	142
1-3-5-trimethylbenzene	45207	142
1-2-4-trimethylbenzene	45208	142
n-propylbenzene	45209	142
Isopropylbenzene	45210	142

<b>Compound</b>	<b>Parameter Code</b>	<b>Method Code</b>
o-ethyltoluene	45211	142
m-ethyltoluene	45212	142
p-ethyltoluene	45213	142
m-diethylbenzene	45218	142
p-diethylbenzene	45219	142
Styrene	45220	142
1-2-3-trimethylbenzene	45225	142

The Air district operated the GC at Livermore and San Ramon from April to November in 2019. The ozone and NO/NO<sub>2</sub> monitors operate year-round starting in 2019 at both sites.

## 5.5 PM<sub>2.5</sub> Chemical Speciation Network (CSN)

In 1997, the EPA established national 24-hour and annual standards for fine particles less than or equal to 2.5 microns in diameter, known as PM<sub>2.5</sub>, and required each state and local agency to begin ambient monitoring using Federal Reference Method (FRM) samplers. EPA also established a network of chemical speciation monitors to provide information for the development of control strategies in implementation plans and then to track the success of the plans. This monitoring program is known as the Chemical Speciation Network (CSN).

Speciation monitors provide chemical composition of PM<sub>2.5</sub>, which aides in identification of emissions sources. Some CSN sites were designated as long-term trend sites predominately located in large urban areas. Such sites are part of the Speciation Trends Network (STN) to study longer term trends in the chemical composition of PM<sub>2.5</sub>. Other sites in the CSN program are known as CSN supplemental sites.

STN monitoring has the primary objective of defining concentration trends of the elements, ions, and organic and elemental carbon components of PM<sub>2.5</sub>. In January 1999, a PM<sub>2.5</sub> FRM sampler was installed in San Jose and the first year of data showed exceedances of the national standard. Consequently, EPA requested that a Met One Spiral Ambient Speciation Sampler (SASS) be installed at the San Jose monitoring site (which was located on Fourth Street at the time) as part of the STN program because the site is in a major urban area. The site was relocated to Jackson Street in 2002. The sampler operates 24 hours, from midnight to midnight, and samples are collected on a 1:3 schedule.

In April 2005, the Clean Air Scientific Advisory Committee supported changes to the EPA PM<sub>2.5</sub> speciation network to improve comparability with the rural Interagency Monitoring of Protected Visual Environments (IMPROVE) PM<sub>2.5</sub> carbon concentration data. The EPA process, designed to achieve this comparability, included replacing the carbon sampling method with the IMPROVE carbon Thermal Optical Reflectance (TOR) analysis method instead of the Thermal Optical Transmittance (TOT) method. Additionally, the EPA also requested the manufacturer of the IMPROVE sampler, URG Corporation, to modify the sampler to incorporate mass flow control versus fixed-orifice flow control. This effort resulted in a new instrument called the URG-3000N Sequential Particulate Speciation System. In the Bay Area, the Air District began operating the URG 3000 to collect PM<sub>2.5</sub> carbon concentrations at San Jose starting on April 1, 2009, while continuing to operate the SASS sampler to collect all the other compounds.

Filters collected by the SASS and URG-3000 samplers are later analyzed using energy-dispersive X-ray fluorescence, ion chromatography, and thermal/optical analysis

techniques to measure metals, anions and cations, and carbon (elemental and organic) components, respectively. The STN filters are analyzed by an EPA national contract laboratory. The sixty-five chemical species measured are listed in Table 5-4, and can be viewed on the EPA's AirData website at [http://www.epa.gov/airdata/ad\\_maps.html](http://www.epa.gov/airdata/ad_maps.html).

### 5.5.1 BAAQMD Supplemental PM<sub>2.5</sub> Speciation Network Program

The Air District added SASS samplers to existing air monitoring sites at Vallejo and Livermore in 2008 and at the Oakland West station in 2009. These samplers are not part of the national CSN program but contribute to local monitoring objectives. Vallejo and Livermore were selected for sampling because there was an interest in determining the sources of PM<sub>2.5</sub> on days that exceed the standard at those sites, since exceedances often occur on days when the air flow is from the Central Valley. These sites may have a different PM<sub>2.5</sub> composition than at San Jose – Jackson. Oakland West was selected because it is downwind of the Port of Oakland, a major source of diesel particulate matter. The Air District operates these samplers on a 1:6 schedule. Prior to 2015, DRI provided the filters, did the analysis, and submitted the data to AQS; and the filters were also analyzed for palladium, thallium and uranium. Starting with data collected in January 2015, the Air District's laboratory staff have prepared the filters and performed the analysis.

Table 5-4. PM<sub>2.5</sub> Speciation Measurements at Air District Sites in 2019

Compound	Parameter Code at San Jose	Parameter Code at Other Sites	Method Code at San Jose	Method Code at Other Sites
<b>Metals</b>				
Antimony	88102	88102	811	811
Arsenic	88103	88103	811	811
Aluminum	88104	88104	811	811
Barium	88107	88107	811	811
Bromine	88109	88109	811	811
Cadmium	88110	88110	811	811
Calcium	88111	88111	811	811
Chromium	88112	88112	811	811
Cobalt	88113	88113	811	811
Copper	88114	88114	811	811
Chlorine	88115	88115	811	811
Cerium	88117	88117	811	811
Cesium	88118	88118	811	811
Europium	88121	88121	811	811

<b>Compound</b>	<b>Parameter Code at San Jose</b>	<b>Parameter Code at Other Sites</b>	<b>Method Code at San Jose</b>	<b>Method Code at Other Sites</b>
Gallium	88124	88124	811	811
Gold	88143	88143	811	811
Hafnium	88127	88127	811	811
Iron	88126	88126	811	811
Indium	88131	88131	811	811
Iridium	88133	88133	811	811
Lanthanum	88146	88146	811	811
Lead	88128	88128	811	811
Manganese	88132	88132	811	811
Molybdenum	88134	88134	811	811
Magnesium	88140	88140	811	811
Mercury	88142	88142	811	811
Nickel	88136	88136	811	811
Niobium	88147	88147	811	811
Palladium <sup>1</sup>	-	88151	-	811
Phosphorous	88152	88152	811	811
Potassium	88180	88180	811	811
Rubidium	88176	88176	811	811
Samarium	88162	88162	811	811
Scandium	88163	88163	811	811
Selenium	88154	88154	811	811
Silicon	88165	88165	811	811
Silver	88166	88166	811	811
Sodium	88184	88184	811	811
Strontium	88168	88168	811	811
Sulfur	88169	88169	811	811
Tantalum	88170	88170	811	811
Terbium	88172	88172	811	811
Thallium <sup>1</sup>	-	88173	-	811
Tin	88160	88160	811	811
Titanium	88161	88161	811	811
Tungsten	88186	88186	811	811
Uranium <sup>1</sup>	-	88179	-	811
Vanadium	88164	88164	811	811
Yttrium	88183	88183	811	811
Zinc	88167	88167	811	811
Zirconium	88185	88185	811	811
<b>Anions and Cations</b>				
Ammonium Cation	88301	88301	812	812



<b>Compound</b>	<b>Parameter Code at San Jose</b>	<b>Parameter Code at Other Sites</b>	<b>Method Code at San Jose</b>	<b>Method Code at Other Sites</b>
Sodium Cation	88302	88302	812	812
Chloride Anion	88203	88203	812	812
Sulfate Anion	88403	88403	812	812
Potassium Cation	88303	88303	812	812
Nitrate Anion	88306	88306	812	812
<b>Organic and Elemental Carbon</b>				
Total Organic Carbon (sum of the OC Fractions below)	88370	88320	838	815
Elemental Carbon Fraction 1 (carbon released at 550°C in 10% oxygen/90% helium gas)	88383	88329	841	814
Elemental Carbon Fraction 2 (carbon released at 700°C in 10% oxygen/90% helium gas)	88384	88330	841	814
Elemental Carbon Fraction 3 (carbon released at 800°C in 10% oxygen/90% helium gas)	88384	88331	841	814
Organic Carbon Fraction 1 (carbon released at 120°C in helium gas)	88374	88324	841	814
Organic Carbon Fraction 2 (carbon released at 250°C in helium gas)	88375	88325	841	814
Organic Carbon Fraction 3 (carbon released at 450°C in helium gas)	88376	88326	841	814
Organic Carbon Fraction 4 (carbon released at 550°C in helium gas)	88377	88327	841	814

<sup>1</sup> Elements measured only at Vallejo, Livermore, and Oakland West.

## 5.6 Toxics Program

The Clean Air Act Amendments of 1990 required EPA to set emission standards for major sources of Hazardous Air Pollutants (HAPs). The Act also required EPA to assess the risks to human health from HAPs. As of 2012 EPA had listed 187 compounds as HAPs and are known to cause or are suspected of causing cancer, birth defects, reproduction problems, and other serious illnesses. Exposure time to certain levels of some HAPs can cause difficulty in breathing, nausea, or other illnesses and can even cause death.

Toxic pollutants (HAPs) are emitted daily by industrial and chemical manufacturing processes, commercial activities, refinery operations, gasoline marketing, and motor vehicles within the Bay Area. Ambient concentrations vary by proximity to sources and current meteorological conditions.


The Air District established an ambient air toxics monitoring program with the objectives of:

- Establishing trends and evaluating the effectiveness of HAP reduction strategies.
- Characterizing ambient concentrations in local areas.
- Providing data to support and evaluate dispersion and deposition models.
- Providing data to the scientific community to support studies to reduce uncertainty about the relationships between ambient levels of HAPs, actual human exposure to air toxics, and health effects from such exposures.

**Error! Reference source not found.** is a map of the 23 toxics monitoring sites operating in 2018. They are located at existing Air District monitoring stations to measure a wide range of contaminant levels throughout the Bay Area. The sites are generally located in major population centers or downwind of major industrial sources such as refineries. There is also an ambient background site at Fort Cronkhite.

Air samples are collected at Air District toxics monitoring sites for a 24-hour period on a 1:12 schedule. At San Jose Jackson, the sampling schedule was on a 1:6 as part of the NATTS program through August 6, 2018 and was changed to a 1:12 starting August 18, 2018 because this site is no longer part of the NATTS program. A 1:12 schedule allows samples to be taken on a different day of the week over the course of months. This is the same schedule EPA and CARB use for their toxics monitoring programs, thereby allowing Bay Area toxics concentrations to be compared to concentrations measured elsewhere across the country.

Gaseous (VOC) toxics are collected in 6-liter SUMMA stainless steel canisters using Xontech 910 samplers. The sampler continuously collects an ambient air sample for 24-hours to ensure capturing transient and intermittent toxic releases. Since 2012, samples have been analyzed using gas chromatography mass spectrometry.

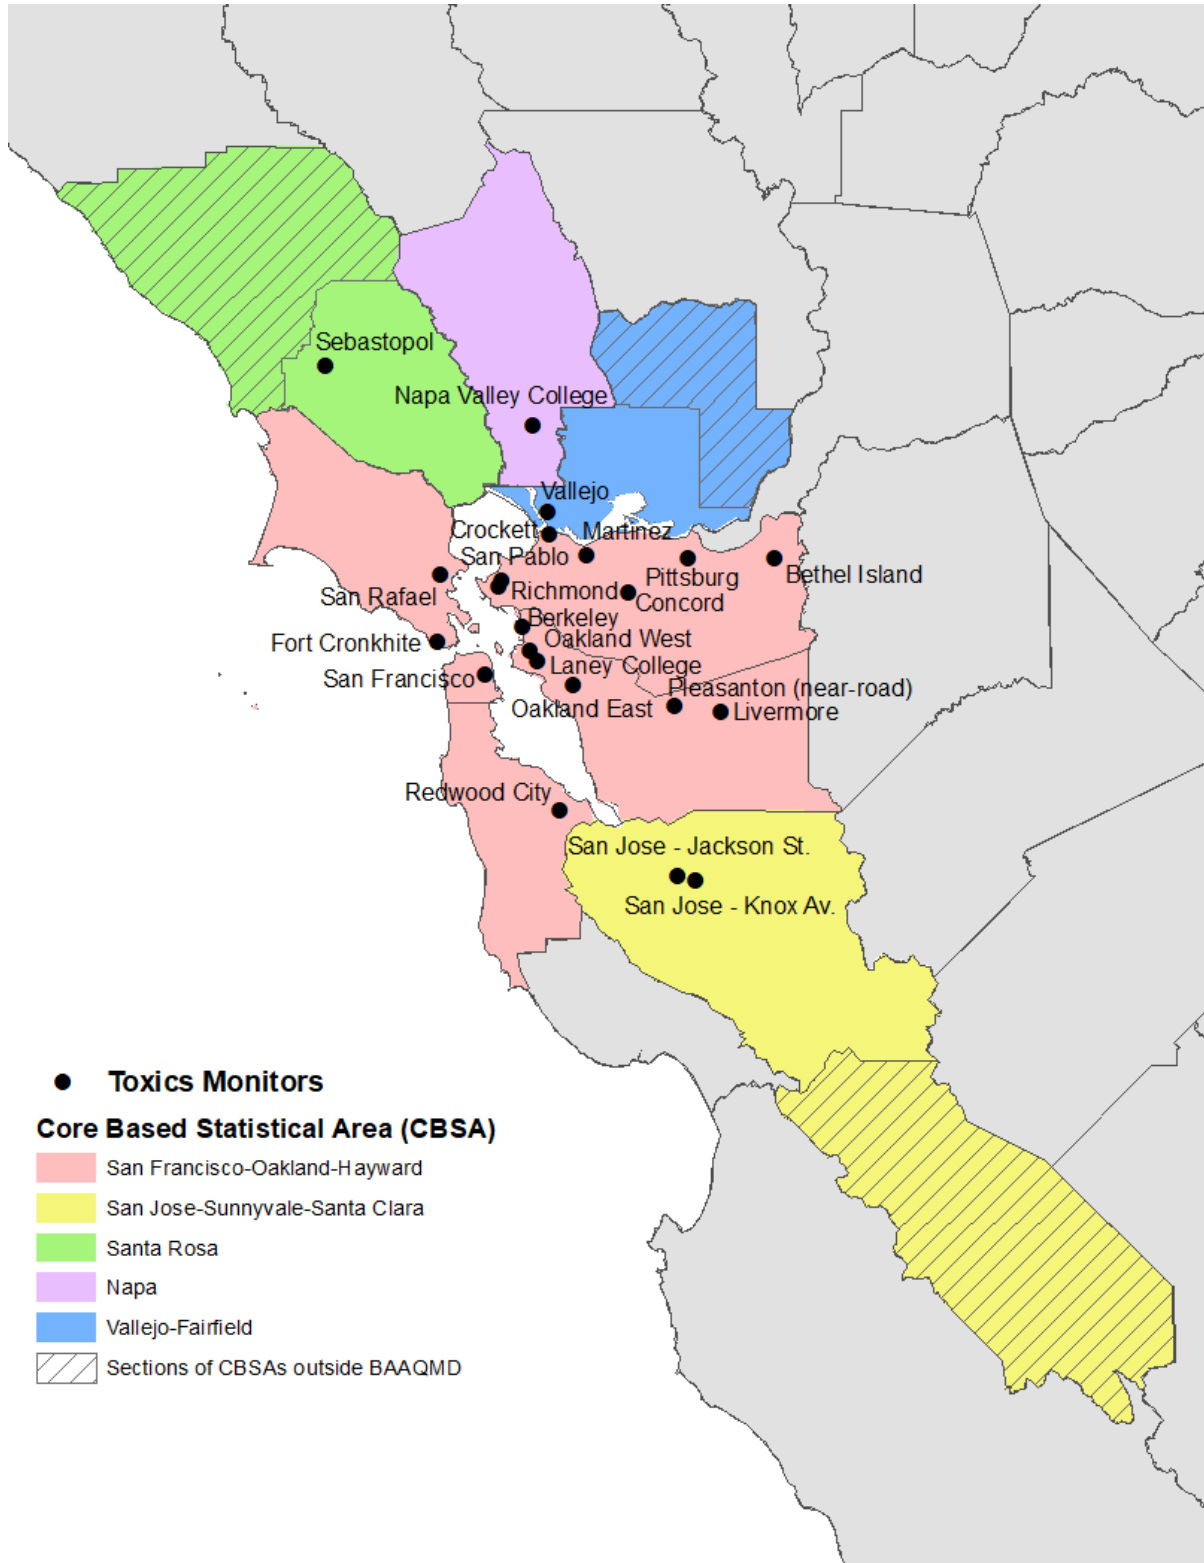

**Figure 5-4.** Map of Air District Toxics Monitoring Sites in 2019

Both the Air District and CARB have toxics monitoring programs in the Bay Area. CARB conducts toxics monitoring on a 1:12 schedule at two sites: San Francisco and San Jose. CARB supplies the canisters and performs the laboratory analyses, while Air District staff operates the CARB sampler and ships the canisters to CARB. Because the Air District also does toxics monitoring at San Francisco and San Jose, the two sets of data allow calculation of the measurement precision at these sites, and by extrapolation, an estimate of the precision of the toxics measurement program.

For Quality Assurance purposes, once a quarter at San Francisco, an additional canister sample is taken on a scheduled sample day using a collocated sampler. Both samples are analyzed by the Air District laboratory, and the results allow an additional measure of precision. Additionally, at least one canister per month is chosen at random for a second analysis. The results are submitted to AQS for both the San Francisco collocated sample and the randomly selected replicate analysis.

From each canister sample, the Air District laboratory analyzes for the 22 gaseous toxic compounds shown in Table 5-5 from canister samples collected using a gas chromatography mass spectrometry instrument. The compounds selected for analysis were those that had high toxicity or were known to have high emissions in the Bay Area, or a combination of the two. Another consideration was whether the current methodology could accurately detect a compound at reasonable expense, based on previous CARB studies. Some compounds, such as carbon tetrachloride, are measured because their concentration in the ambient air does not change much over time. This is useful because carbon tetrachloride or other similar, stable compounds can be used for quality control purposes. If the measurement of such a control is unusually high or low, there may be a problem in the sampling, transport, storage, or analysis procedures.

Table 5-5. List of Toxic Compounds Measured by the Air District in 2019

<b>Compound</b>	<b>Parameter Code</b>	<b>Method Code</b>
1,3-Butadiene	43218	210
Acetone	43551	210
Acetonitrile	43702	210
Acrylonitrile	43704	210
Benzene	45201	210
Carbon tetrachloride	43804	210
Chloroform	43803	210
Dichloromethane	43802	210
Ethyl alcohol	43302	210

<b>Compound</b>	<b>Parameter Code</b>	<b>Method Code</b>
Ethylbenzene	45203	210
Ethylene dibromide	43843	210
Ethylene dichloride	43815	210
Freon 113	43207	210
m/p Xylene	45109	210
Methyl chloroform	43814	210
Methyl ethyl ketone	43552	210
o-Xylene	45204	210
Tetrachloroethylene	43817	210
Toluene	45202	210
Trichloroethylene	43824	210
Trichlorofluoromethane	43811	210
Vinyl chloride	43860	210

### **5.6.1 Additional Toxics Monitoring at San Jose**

In addition to the compounds listed in Table 5-5, formaldehyde and acetaldehyde are measured at San Jose on a 1:6 schedule through August 6, 2018 and on a 1:12 schedule starting August 18, 2018 through present. These compounds are highly reactive and cannot be accurately measured using a canister sample. Instead, they are collected on a chemically treated cartridge using a Xontech 924 sampler. Samples are analyzed at the Air District laboratory using High Performance Liquid Chromatography.

Metals are also measured at San Jose. In addition, summary toxics data are available from the EPA's AirData website at: <http://www.epa.gov/airdata/>.

## **Appendices A through G**

## APPENDIX A. OZONE MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD



BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT

June 4, 2014

Mr. Michael J. Gilroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940

Dear Mr. Gilroy:

The Bay Area Air Quality Management District has signed the Ozone monitoring agreement as described in your letter of May 23, 2014 (attached). We will continue to operate the Ozone monitors at San Jose, Los Gatos, Gilroy, and San Martin as stated in your letter. We will advise you well in advance if any of these monitors are shutdown or moved to another location.

Sincerely,

A handwritten signature in blue ink, appearing to read "Eric D. Stevenson".

Eric D. Stevenson  
Director, Technical Services Division

Enclosure





**MBUAPCD**

Monterey Bay Unified Air Pollution Control District  
Serving Monterey, San Benito, and Santa Cruz Counties

24580 Silver Cloud Court  
Monterey, CA 93940

PHONE: (831) 647-9411 • FAX: (831) 647-8501

May 23, 2014

Mr. Eric D. Stevenson  
Director, Technical Services Division  
Bay Area Air Quality Management District  
939 Ellis Street  
San Francisco, CA 94109

Subject: Shared Ozone Monitoring Responsibilities

Dear Mr. Stevenson:

For Ozone monitoring in the San Jose-Sunnyvale-Santa Clara Metropolitan Statistical Area (MSA), both of our agencies are required to meet the full minimum monitoring requirements of 40 CFR Part 58 Appendix D, section (2)(e) in the absence of an Ozone monitoring agreement. The Monterey Bay Unified Air Pollution Control District (MBUAPCD) currently operates one SLAMS Ozone monitor in this MSA (at Hollister) but two monitors are required. Therefore, MBUAPCD would like this letter to serve as a monitoring agreement between our two agencies.

The MBUAPCD requests BAAQMD reply to this letter confirming agreement to continue operation of the SLAMS Ozone monitors at San Jose, Los Gatos, Gilroy, and San Martin. Both agencies will advise each other if changes to the instruments listed below are planned.

	AQS#	Parameter	Method	POC
San Jose	060850005	44201	047	1
Los Gatos	060851001	44201	047	1
Gilroy	060850002	44201	047	1
San Martin	060852006	44201	047	1
Hollister	060690002	44201	047	1

Sincerely,

Michael J. Gilroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940  
(831) 647-9411

## APPENDIX B. APPENDIX B. PM<sub>10</sub> MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD



BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT

January 14, 2013

Mr. William Chevalier  
Supervising Air Monitoring Specialist  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940

Dear Mr. Chevalier:

During a recent review of the Annual Network Report for the Bay Area Air Quality Management District (BAAQMD), EPA Region 9 pointed out that we do not have a written agreement to share minimum monitoring requirements with neighboring Air Districts. For PM<sub>10</sub> monitoring in the San Jose-Sunnyvale-Santa Clara Metropolitan Statistical Area (MSA), both of our agencies are required to meet the full minimum monitoring requirements of 40 CFR Part 58 Appendix D, section (2)(e) in the absence of a PM<sub>10</sub> monitoring agreement.

The San Jose-Sunnyvale-Santa Clara MSA must have two SLAMS PM<sub>10</sub> monitors to meet EPA minimum monitoring requirements. The BAAQMD operates one SLAMS PM<sub>10</sub> monitor at San Jose and will continue to operate this instrument indefinitely.

The BAAQMD requests Monterey Bay Unified Air Pollution Control District reply to this letter confirming agreement to continue operating the SLAMS PM<sub>10</sub> monitor at Hollister. As part of the agreement, both agencies will advise each other if changes to the instruments (as shown below) are planned.

	AQS#	Parameter	Method	POC
San Jose	060850005	81102	127	1
Hollister	060690002	81102	122	3

Sincerely,

Eric D. Stevenson  
Director, Technical Services Division

## APPENDIX C. NO<sub>2</sub> MONITORING AGREEMENT BETWEEN BAAQMD AND MBUAPCD



BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT

June 4, 2014

Mr. Michael J. Gilroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940

Dear Mr. Gilroy:

The Bay Area Air Quality Management District has signed the NO<sub>2</sub> monitoring agreement as described in your letter of May 23, 2014 (attached). We will continue to operate the NO<sub>2</sub> monitor at San Jose as stated in your letter. We will advise you well in advance if this monitor is shutdown or moved to another location.

Sincerely,



Eric D. Stevenson  
Director, Technical Services Division

Enclosure



**MBUAPCD**

Monterey Bay Unified Air Pollution Control District  
Serving Monterey, San Benito, and Santa Cruz Counties

24580 Silver Cloud Court  
Monterey, CA 93940  
PHONE: (831) 647-9411 • FAX: (831) 647-8501

May 23, 2014

Mr. Eric D. Stevenson  
Director, Technical Services Division  
Bay Area Air Quality Management District  
939 Ellis Street  
San Francisco, CA 94109

Subject: Shared NO/NO<sub>2</sub>/NO<sub>x</sub> Monitoring Responsibilities

Dear Mr. Stevenson:

40 CFR Part 58 Appendix D, section (2)(e), requires air monitoring of oxides of nitrogen to be performed to meet minimum federal requirement for the San Jose-Sunnyvale-Santa Clara Metropolitan Statistical Area (MSA). The Monterey Bay Unified Air Pollution Control District (MBUAPCD) currently does not operate any SLAMS NO<sub>2</sub> monitors in this MSA and would like this letter to serve as a monitoring agreement between our two agencies.

The MBUAPCD requests the Bay Area Air Quality Management District reply to this letter confirming agreement to continue operation of the SLAMS NO<sub>2</sub> monitor at San Jose and advise MBUAPCD if changes to this instrument are planned.

	AQS#	Parameter	Method	POC
San Jose	060850005	42602	074	1

Sincerely,

Michael J. Giffroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940  
(831) 647-9411

**APPENDIX D. CO, NO<sub>2</sub>, AND PM<sub>2.5</sub> NEAR-ROAD MONITORING  
AGREEMENT BETWEEN BAAQMD AND MBUAPCD**



BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT

May 14, 2015

Mr. Michael J. Gilroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940

Dear Mr. Gilroy:

The Bay Area Air Quality Management District has signed the shared near-road CO, NO<sub>2</sub> and PM<sub>2.5</sub> monitoring agreement as described in your letter of May 13, 2015 (attached). We will continue to operate these monitors at the San Jose Knox monitoring site (060850006) as stated in your letter. We will advise you in advance if any of these monitors are shutdown or moved to another location.

Sincerely,

A handwritten signature in black ink, appearing to read "Eric D. Stevenson".

Eric D. Stevenson  
Director, Meteorology, Measurement and Rules Division

Enclosure



**MBUAPCD**

Monterey Bay Unified Air Pollution Control District  
Serving Monterey, San Benito, and Santa Cruz Counties

24580 Silver Cloud Court  
Monterey, CA 93940

PHONE: (831) 647-9411 • FAX: (831) 647-8501

May 13, 2015

Mr. Eric D. Stevenson  
Director, Technical Services Division  
Bay Area Air Quality Management District  
939 Ellis Street  
San Francisco, CA 94109

Subject: Shared Near-Road CO, NO<sub>2</sub>, and PM<sub>2.5</sub> Monitoring Responsibilities

Dear Mr. Stevenson:

40 CFR Part 58 Subparts 58.10(a)(7), 58.13(e)(1), and Appendix D section 4.3.1, requires near-road monitoring of CO, NO<sub>x</sub>, and PM<sub>2.5</sub> to be performed to meet minimum federal requirements for the San Jose-Sunnyvale-Santa Clara Core Based Statistical Area (CBSA), 41940. The Bay Area Air Quality Management District (BAAQMD) established a near-road monitor in San Jose on September 1, 2014 and will take responsibility for meeting these near-road requirements as they currently exist. The Monterey Bay Unified Air Pollution Control District (MBUAPCD) currently does not operate any Near-Road CO, NO<sub>2</sub>, and PM<sub>2.5</sub> monitors in this MSA and would like this letter to serve as a monitoring agreement between our two agencies.

The MBUAPCD requests the Bay Area Air Quality Management District reply to this letter confirming agreement to continue operation of the Near-Road CO, NO<sub>2</sub>, and PM<sub>2.5</sub> monitors at San Jose-Knox Avenue and advise MBUAPCD if changes to this instrument are planned.

	AQS#	Parameter	Method	POC
San Jose	060850006	42101	054	1
San Jose	060850006	42602	074	1
San Jose	060850006	88101	170	1

Sincerely,

Michael J. Gilroy  
Deputy Air Pollution Control Officer  
Monterey Bay Unified Air Pollution Control District  
24580 Silver Cloud Court  
Monterey, CA 93940  
(831) 647-9411





## APPENDIX E. APPROVAL TO END MONITORING OF NO<sub>y</sub> AT THE SAN JOSE NCore SITE



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
RESEARCH TRIANGLE PARK, NC 27711

October 30, 2017

OFFICE OF  
AIR QUALITY PLANNING  
AND STANDARDS

Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street, Suite 600  
San Francisco, CA 94105

Dear Mr. Stevenson:

This letter transmits our approval of the Bay Area Air Quality Management District (BAAQMD) request to shut down the agencies' NO<sub>y</sub> monitor in concert with continued operation of a NO<sub>x</sub> monitor at the San Jose-Jackson Street NCore station (AQS site ID: 06-085-0005). This request is being made so that the NO<sub>y</sub> monitor can be installed and operated at the proposed PAMS station in Livermore, California (AQS site ID: 06-001-0007). Requests to allow monitoring for NO<sub>x</sub> instead of NO<sub>y</sub> at NCore stations are covered in our monitoring regulations (see Appendix D to Part 58, Section 3, (b)(1)). According to these rules, a waiver for measuring NO<sub>x</sub> in lieu of NO<sub>y</sub> must be approved by the Environmental Protection Agency's (EPA) Administrator. This authority has been delegated to the Director of the Air Quality Assessment Division in EPA's Office of Air Quality Planning and Standards.

In considering your request to operate NO<sub>x</sub> in lieu of NO<sub>y</sub> at the San Jose-Jackson Street NCore station, we worked with EPA Region 9 on an evaluation of the NO<sub>y</sub> and NO<sub>x</sub> data at the San Jose-Jackson Street station and a review of the rationale for why the proposed PAMS station is better suited for NO<sub>y</sub> measurements. After careful consideration of your request to move the NO<sub>y</sub> monitor to the proposed PAMS station in Livermore and operate NO<sub>x</sub> at San Jose-Jackson Street we are pleased to approve the shut-down of NO<sub>y</sub> at the San Jose-Jackson Street NCore station. We note that PAMS measurements are required to operate minimally during June, July, and August, while NCore measurements are required to operate year-round. Since the Livermore site would be the only BAAQMD location with both NO<sub>y</sub> and true NO<sub>2</sub>, we expect that you will operate these measurements year-round. Let us know if this is not possible.

The strength of the rationale to prioritize operation of NO<sub>y</sub> at Livermore over San Jose-Jackson Street is that it allows for collocating NO<sub>y</sub> with a true NO<sub>2</sub> monitor at Livermore. This collocation of NO<sub>y</sub> and true NO<sub>2</sub> will ensure that calculations of NO<sub>z</sub> are made with the most appropriate monitoring technologies. This is consistent with our authority to allow such a waiver since differences between NO<sub>y</sub> and true NO<sub>2</sub> + NO are expected to be larger than differences between NO<sub>y</sub> and NO<sub>x</sub> chemiluminescence monitors, as is the case for the existing monitors at San Jose-Jackson Street.

Internet Address (URL) • <http://www.epa.gov>

Recycled/Recyclable • Printed with Vegetable Oil Based Inks on Recycled Paper (Minimum 25% Postconsumer)



If you have any questions regarding this letter, please feel free to contact me at (415) 972-3851, or Anna Mebust of my staff at (415) 972-3265.

cc: (via email): Tim Hanley, OAQPS



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
RESEARCH TRIANGLE PARK, NC 27711

October 30, 2017

OFFICE OF  
AIR QUALITY PLANNING  
AND STANDARDS

Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street, Suite 600  
San Francisco, CA 94105

Dear Mr. Stevenson:

This letter transmits our approval of the Bay Area Air Quality Management District (BAAQMD) request to shut down the agencies' NOy monitor in concert with continued operation of a NOx monitor at the San Jose-Jackson Street NCore station (AQS site ID: 06-085-0005). This request is being made so that the NOy monitor can be installed and operated at the proposed PAMS station in Livermore, California (AQS site ID: 06-001-0007). Requests to allow monitoring for NOx instead of NOy at NCore stations are covered in our monitoring regulations (see Appendix D to Part 58, Section 3. (b)(1)). According to these rules, a waiver for measuring NOx in lieu of NOy must be approved by the Environmental Protection Agency's (EPA) Administrator. This authority has been delegated to the Director of the Air Quality Assessment Division in EPA's Office of Air Quality Planning and Standards.

In considering your request to operate NOx in lieu of NOy at the San Jose-Jackson Street NCore station, we worked with EPA Region 9 on an evaluation of the NOy and NOx data at the San Jose-Jackson Street station and a review of the rationale for why the proposed PAMS station is better suited for NOy measurements. After careful consideration of your request to move the NOy monitor to the proposed PAMS station in Livermore and operate NOx at San Jose-Jackson Street we are pleased to approve the shut-down of NOy at the San Jose-Jackson Street NCore station. We note that PAMS measurements are required to operate minimally during June, July, and August, while NCore measurements are required to operate year-round. Since the Livermore site would be the only BAAQMD location with both NOy and true NO<sub>2</sub>, we expect that you will operate these measurements year-round. Let us know if this is not possible.


The strength of the rationale to prioritize operation of NOy at Livermore over San Jose-Jackson Street is that it allows for collocating NOy with a true NO<sub>2</sub> monitor at Livermore. This collocation of NOy and true NO<sub>2</sub> will ensure that calculations of NOz are made with the most appropriate monitoring technologies. This is consistent with our authority to allow such a waiver since differences between NOy and true NO<sub>2</sub> + NO are expected to be larger than differences between NOy and NOx chemiluminescence monitors, as is the case for the existing monitors at San Jose-Jackson Street.

Internet Address (URL) • <http://www.epa.gov>

Recycled/Recyclable • Printed with Vegetable Oil Based Inks on Recycled Paper (Minimum 25% Postconsumer)

Thank you for your program's efforts in working through the issue of optimizing your network to meet multiple needs at NCore and PAMS. For any technical questions on NCore, you may contact Tim Hanley at [hanley.tim@epa.gov](mailto:hanley.tim@epa.gov) and 919-541-4417. For technical questions on PAMS, you may contact Kevin Cavender at [cavender.kevin@epa.gov](mailto:cavender.kevin@epa.gov) and 919-541-2364.

Sincerely,



Richard A. Wayland  
Director  
Air Quality Assessment Division

cc: Matthew J. Lakin, EPA Region 9



**BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT**

**ALAMEDA COUNTY**  
Tom Bates  
Scott Haggerty  
Nate Miley  
(Chair)  
Tim Gibrani

**CONTRA COSTA COUNTY**  
John Gioia  
David Hudson  
Mary Piepho  
Mark Ross

**MARIN COUNTY**  
Susan Adams

**NAPA COUNTY**  
Brad Wagenknecht

**SAN FRANCISCO COUNTY**  
John Avalos  
Edwin M. Lee  
Eric Mar  
(Secretary)

**SAN MATEO COUNTY**  
Carole Groom  
(Vice-Chair)  
Carol Klatt

**SANTA CLARA COUNTY**  
Cindy Chavez  
Ash Kalra  
Liz Kniss  
Jan Pepper

**SOLANO COUNTY**  
James Spelling

**SONOMA COUNTY**  
Teresa Barnett  
Shirlee Zane

Jack P. Broadbent  
EXECUTIVE OFFICER/PA/CO

March 3, 2014

Ms. Meredith Kurpius, Ph.D.  
Manager, Air Quality Analysis Office  
United States Environmental Protection Agency, Region IX  
75 Hawthorne Street  
San Francisco, CA 94105-3901

Dear Ms. Kurpius:

Since January 2011, the Bay Area Air Quality Management District (Air District) has been operating a federally mandated NOy instrument as part of EPA NCore requirements at our San Jose NCore site; AQS ID 06-085-0005.

Hourly average data from this monitor have been submitted to the EPA AQS data base using the required method code 599 and parameter code 42600.

Analysis of 24 hourly NOx vs. NOy averages indicate statistically insignificant differences between NOx and NOy measurements as demonstrated in the three figures (24 hr NOx vs NOy correlation, by year) included below. To enable more efficient utilization of both fiscal and personnel resources within the Air District Air Monitoring Section, we are requesting that the EPA Administrator grant a waiver permitting NOx monitoring to be substituted for the required NOy monitoring at the Air District NCore site, as allowed in *40CFR Part 58 Appendix D.3: Design Criteria for NCore Sites*.

The EPA NCore requirements from 40CFR Part 58 Appendix D.3: Design Criteria for NCore Sites as last amended on Dec. 27<sup>th</sup> 2010 includes the following in paragraph 3 (b) (1);

*Although the measurement of NOy is required in support of a number of monitoring objectives, available commercial instruments may indicate little difference in their measurement of NOy compared to the conventional measurement of NOx, particularly in areas with relatively fresh sources of nitrogen emissions. Therefore, in areas with negligible expected difference between NOy and NOx measured concentrations, the Administrator may allow for waivers that permit NOx monitoring to be substituted for the required NOy monitoring at applicable NCore sites.*

All data represented in the figures below is available for further analysis in the EPA AQS data base, or can be provided upon request if independent verification by EPA is desired. We propose to close this monitor immediately upon receipt of the Administrator's letter providing the requested waiver.


Meredith Kurpius  
Page 2

3/3/14

---

Please contact Glen Colwell at (415) 749-4672 if you have any questions or concerns.

Sincerely,



Eric D. Stevenson  
Director of Technical Services

cc: K. Hoag, EPA Region 9  
G. Yoshimura, EPA Region 9  
E. Felix, EPA Region 9

cc: K. Malone,  
M. Flagg, EPA Region 9

Figure 1 – NCore BAAQMD San Jose: NOx vs. NOy 2013 24 Hr Correlation: R2 = 0.995

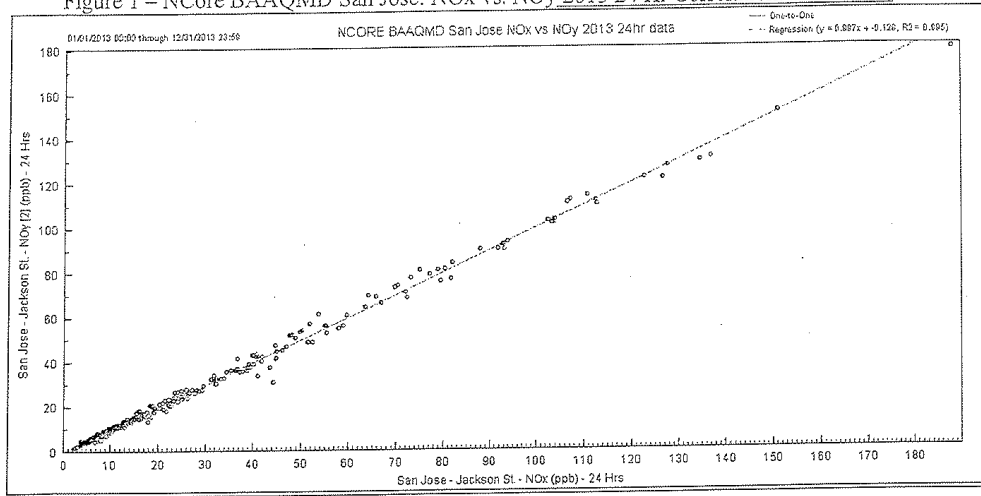


Figure 2 – NCore BAAQMD San Jose: NOx vs. NOy 2012 24 Hr Correlation: R2 = 0.994


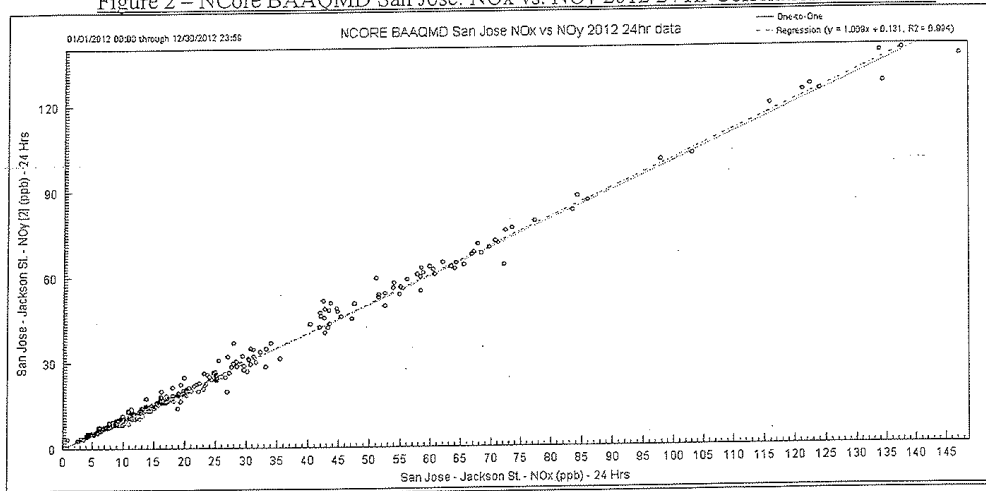


Figure 3 – NCore BAAQMD San Jose: NOx vs. NOy 2011 24 Hr Correlation: R2 = 0.996



## APPENDIX F. EPA'S APPROVAL TO END NO<sub>y</sub> MONITORING AT SAN JOSE N CORE SITE

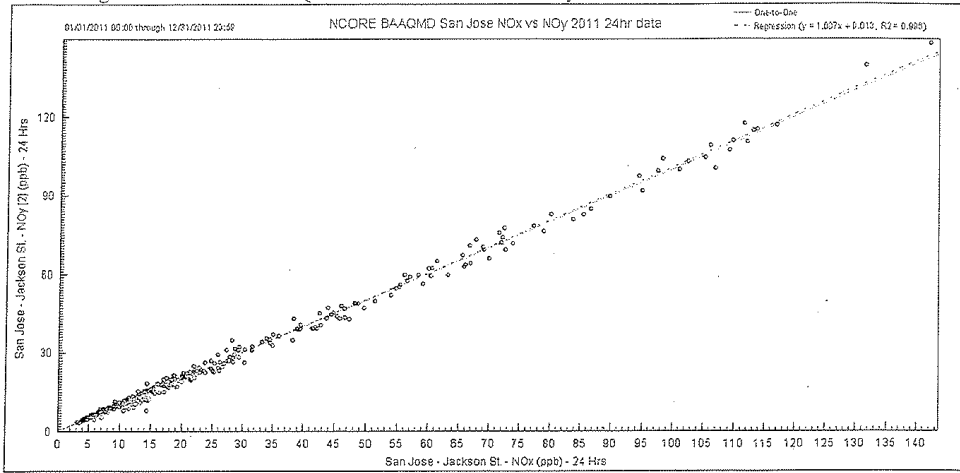

UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
RESEARCH TRIANGLE PARK, NC 27711

October 30, 2017

OFFICE OF  
AIR QUALITY PLANNING  
AND STANDARDS

Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street, Suite 600  
San Francisco, CA 94105

Dear Mr. Stevenson:

This letter transmits our approval of the Bay Area Air Quality Management District (BAAQMD) request to shut down the agencies' NO<sub>y</sub> monitor in concert with continued operation of a NO<sub>x</sub> monitor at the San Jose-Jackson Street NCore station (AQS site ID: 06-085-0005). This request is being made so that the NO<sub>y</sub> monitor can be installed and operated at the proposed PAMS station in Livermore, California (AQS site ID: 06-001-0007). Requests to allow monitoring for NO<sub>x</sub> instead of NO<sub>y</sub> at NCore stations are covered in our monitoring regulations (see Appendix D to Part 58, Section 3. (b)(1)). According to these rules, a waiver for measuring NO<sub>x</sub> in lieu of NO<sub>y</sub> must be approved by the Environmental Protection Agency's (EPA) Administrator. This authority has been delegated to the Director of the Air Quality Assessment Division in EPA's Office of Air Quality Planning and Standards.

In considering your request to operate NO<sub>x</sub> in lieu of NO<sub>y</sub> at the San Jose-Jackson Street NCore station, we worked with EPA Region 9 on an evaluation of the NO<sub>y</sub> and NO<sub>x</sub> data at the San Jose-Jackson Street station and a review of the rationale for why the proposed PAMS station is better suited for NO<sub>y</sub> measurements. After careful consideration of your request to move the NO<sub>y</sub> monitor to the proposed PAMS station in Livermore and operate NO<sub>x</sub> at San Jose-Jackson Street we are pleased to approve the shut-down of NO<sub>y</sub> at the San Jose-Jackson Street NCore station. We note that PAMS measurements are required to operate minimally during June, July, and August, while NCore measurements are required to operate year-round. Since the Livermore site would be the only BAAQMD location with both NO<sub>y</sub> and true NO<sub>2</sub>, we expect that you will operate these measurements year-round. Let us know if this is not possible.

The strength of the rationale to prioritize operation of NO<sub>y</sub> at Livermore over San Jose-Jackson Street is that it allows for collocating NO<sub>y</sub> with a true NO<sub>2</sub> monitor at Livermore. This collocation of NO<sub>y</sub> and true NO<sub>2</sub> will ensure that calculations of NO<sub>z</sub> are made with the most appropriate monitoring technologies. This is consistent with our authority to allow such a waiver since differences between NO<sub>y</sub> and true NO<sub>2</sub> + NO are expected to be larger than differences between NO<sub>y</sub> and NO<sub>x</sub> chemiluminescence monitors, as is the case for the existing monitors at San Jose-Jackson Street.


Internet Address (URL) • <http://www.epa.gov>

Recycled/Recyclable • Printed with Vegetable Oil Based Inks on Recycled Paper (Minimum 25% Postconsumer)



Thank you for your program's efforts in working through the issue of optimizing your network to meet multiple needs at NCore and PAMS. For any technical questions on NCore, you may contact Tim Hanley at [hanley.tim@epa.gov](mailto:hanley.tim@epa.gov) and 919-541-4417. For technical questions on PAMS, you may contact Kevin Cavender at [cavender.kevin@epa.gov](mailto:cavender.kevin@epa.gov) and 919-541-2364.

Sincerely,



Richard A. Wayland  
Director  
Air Quality Assessment Division

cc: Matthew J. Lakin, EPA Region 9



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
REGION IX  
75 Hawthorne Street  
San Francisco, CA 94105-3901

OCT 11 2017

**MEMORANDUM**

**SUBJECT:** Request for OAQPS Approval: NO<sub>y</sub> Waiver for the Bay Area Air Quality Management District's San Jose-Jackson NCore Site

**FROM:** Matthew J. Lakin  
Acting Director, Air Division

**TO:** Richard A. Wayland  
Director, Air Quality Assessment Division

I am writing to transmit a request from the Bay Area Air Quality Management District (BAAQMD) for a waiver of the requirement for observations of total reactive nitrogen oxides (NO<sub>y</sub>) at the San Jose-Jackson National Core multi-pollutant monitoring (NCore) site (AQS ID: 06-085-0005). BAAQMD communicated this request in their 2016 Air Monitoring Network Plan (Network Plan), submitted June 29, 2017. As you are aware, 40 CFR 58 Appendix D Section 3(b)(1) allows for the U.S. Environmental Protection Agency (EPA) Administrator to issue waivers to substitute nitrogen oxides (NO<sub>x</sub>) for required NO<sub>y</sub> monitoring at applicable NCore sites, which has been delegated to your office.

NO<sub>y</sub> monitoring is currently required for NCore and will be required for Photochemical Assessment Monitoring Stations (PAMS) beginning in June 2019 for BAAQMD. In Appendix H of their Network Plan, BAAQMD requested a waiver from EPA to locate required PAMS measurements at Livermore (AQS ID: 06-001-0007) rather than at San Jose-Jackson. BAAQMD is requesting this waiver because Livermore is important for regional modeling, as it is the maximum concentration and design value site for the Bay Area ozone (O<sub>3</sub>) nonattainment area. Making Livermore an official PAMS will also allow for better tracking of O<sub>3</sub> precursor trends, since it has operated as an unofficial PAMS for the past seven years. An initial assessment of BAAQMD's request suggests that it meets the criteria in 40 CFR 58 Appendix D Section 5(c) for the waiver. EPA Region 9 intends to address this request through the annual network plan approval.

BAAQMD is requesting a waiver from the NCore requirement for NO<sub>y</sub> at San Jose-Jackson in order to move the NO<sub>y</sub> instrument to Livermore, as part of the required PAMS measurements. Locating NO<sub>y</sub> at Livermore with PAMS rather than at San Jose-Jackson with NCore will allow for collocation of NO<sub>y</sub> with important O<sub>3</sub> precursor measurements. Additionally, BAAQMD has included analysis in their Network Plan, Appendix F, and in previous NO<sub>y</sub> waiver requests, showing little difference between NO<sub>y</sub> and NO<sub>x</sub> concentrations at San Jose-Jackson.

Based on our position on BAAQMD's waiver request to locate PAMS at Livermore, as well as your approval of NO<sub>y</sub> waivers for other agencies under similar circumstances, we recommend that you approve BAAQMD's request for an NO<sub>y</sub> waiver at San Jose-Jackson.

If you have any questions regarding this letter, please feel free to contact me at (415) 972-3851, or Anna Mebust of my staff at (415) 972-3265.

cc: (via email): Tim Hanley, OAQPS

**APPENDIX G. REQUEST AND APPROVAL TO DISCONTINUE LEAD  
MONITORING AT SAN JOSE - JACKSON**



**BAY AREA  
AIR QUALITY**

**MANAGEMENT**

**DISTRICT**

September 14, 2018

Gwen Yoshimura  
Manager, Air Quality Analysis Office  
U.S. EPA Region 9  
75 Hawthorne Street  
San Francisco, CA 94105-3901

RE: Discontinuation of Lead (Pb) monitoring at San Jose-Jackson

Dear Ms. Yoshimura,

**ALAMEDA COUNTY**  
John Bauters  
Russo Cutler  
Scott Haggerty  
Nate Miley

**CONTRA COSTA COUNTY**  
John Gioia  
David Hudson  
(Chair)  
Karen Mitchoff  
Mark Ross

**MARIN COUNTY**  
Katie Rice  
(Vice Chair)

**NAPA COUNTY**  
Brad Wagenknecht

**SAN FRANCISCO COUNTY**  
Tyrone Jue  
Hillary Ronen

**SAN MATEO COUNTY**  
David J. Canepa  
Carole Groom  
Doug Kim

**SANTA CLARA COUNTY**  
Margaret Abe-Koga  
Cindy Chavez  
Liz Kniss  
Rod G. Sinks  
(Secretary)

**SOLANO COUNTY**  
James Spering  
Pete Sanchez

**SONOMA COUNTY**  
Teresa Barrett  
Shirlee Zane

Jack P. Broadbent  
EXECUTIVE OFFICER/APCO

The Bay Area Air Quality Management District (BAAQMD) is requesting approval from the United States Environmental Protection Agency (U.S. EPA) to discontinue Lead (Pb) monitoring at the San Jose-Jackson air monitoring station (Air Quality System number 06-085-0005) in Santa Clara County. Pb monitoring is no longer required at National Core Network (NCore) sites per the Code of Federal Registry, Title 40, Part 58 Appendix D, section 3(b).

An analysis of the Pb-PM<sub>10</sub> data at San Jose-Jackson is included with this request to further justify discontinuing Pb monitoring. FRM/FEM Pb-PM<sub>10</sub> monitoring at San Jose-Jackson began in June 2012. The average of the 2013-2015, 2014-2016, and 2015-2017 design values is 0.01 µg/m<sup>3</sup>, which is well below the National Ambient Air Quality Standard (NAAQS) for Pb of 0.15 µg/m<sup>3</sup>. The analysis indicates a less than 10% probability that Pb design values will exceed 80% of the NAAQS over the next three years.

Non-FRM/FEM Pb-PM<sub>10</sub> monitoring took place at San Jose-Jackson from December 2010 through May 2012. When these data are included with the subsequent FRM/FEM Pb-PM<sub>10</sub> data, the average of the design values in the combined data set is also 0.01 µg/m<sup>3</sup>, which is well below the NAAQS of 0.15 µg/m<sup>3</sup>.

With the approval of U.S. EPA, BAAQMD intends to discontinue Pb monitoring at San-Jose Jackson by the end of 2018.

Sincerely,

Eric D. Stevenson  
Meteorology and Measurement Director

Attachments

cc:



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
REGION IX  
75 Hawthorne Street  
San Francisco, CA 94105-3901

OCT 29 2018

Mr. Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street  
San Francisco, California 94105

Dear Mr. Stevenson:

Thank you for your submission of the Bay Area Air Quality Management District (BAAQMD) *2017 Air Monitoring Network Plan* on July 2, 2018. We have reviewed the submitted document based on the requirements set forth in 40 CFR Part 58. Based on the information provided in the plan, the U.S. Environmental Protection Agency (EPA) approves all portions of the network plan except those specifically identified below. With this plan approval, we also formally approve the following system modification: the closure of the Pb-PM<sub>10</sub> monitor at San Jose-Jackson (AQS ID: 06-085-0005). More information about this approval is included in enclosure B. Please include the request and approval with next year's plan.


Please note that we cannot approve portions of the annual network plan for which the information in the plan is insufficient to judge whether the requirement has been met, or for which the information provided does not meet the requirements as specified in 40 CFR 58.10 and the associated appendices. EPA Region 9 also cannot approve portions of the plan for which the EPA Administrator has not delegated approval authority to the regional offices. The first enclosure (*A. Annual Monitoring Network Plan Checklist*) is the checklist EPA used to review your plan for items that are required to be included in the annual network plan along with our assessment of whether the plan submitted by your agency addresses those requirements. Items highlighted in yellow are those EPA Region 9 is not acting on, as we either lack the authority to approve the specific item, or we have determined that a requirement is either not met or information in the plan is insufficient to judge whether the requirement has been met. Items highlighted in green in enclosure A require attention in order to improve next year's plan.

All comments conveyed via this letter and enclosures should be addressed prior to submittal of next year's annual monitoring network plan to EPA.

Printed on 100% Postconsumer Recycled Paper. Process Chlorine Free.

If you have any questions regarding this letter or the enclosed comments, please feel free to contact me at (415) 947-4134 or Anna Mebust at (415) 972-3265.

Sincerely,



Gwen Yoshimura, Manager  
Air Quality Analysis Office

Enclosures:

- A. Annual Monitoring Network Plan Checklist
- B. EPA Approval of the Discontinuation of Lead Monitoring at San Jose-Jackson

cc (via email): Charles Knoderer, BAAQMD  
Katherine Hoag, BAAQMD  
Jin Xu, California Air Resources Board (CARB)  
Ranjit Bhullar, CARB



## **B. EPA Approval of the Discontinuation of Lead Monitoring at San Jose-Jackson**

This enclosure provides the U.S. Environmental Protection Agency's (EPA's) review and approval for BAAQMD's discontinuation of lead (Pb) monitoring at the San Jose-Jackson NCore site (AQS ID: 06-085-0005).

On September 14, 2018, BAAQMD sent a letter to EPA with a description of this system modification request. BAAQMD began FRM/FEM monitoring for Pb-PM<sub>10</sub> at San Jose-Jackson in June 2012. The highest three-month rolling average measured from the start of monitoring through June 2018 was 0.01 µg/m<sup>3</sup>. As stated in the preamble to the revised monitoring rule (81 FR 17259), EPA anticipated that waiver requests for shutdown of Pb monitoring at urban NCore sites would be received based on three years of data showing design values well below the 2008 Pb National Ambient Air Quality Standards (NAAQS).

EPA approves the shutdown based on a case-by-case approval per 40 CFR 58.14(c). Discontinuance does not compromise data collection needed for implementation of the Pb NAAQS, and the requirements of Appendix D will continue to be met after this monitor is close as Pb monitoring is no longer required at urban NCore sites.

Please include your September 14, 2018 request letter and this response in your next network plan.

## **APPENDIX H. NAPA SITE RELOCATION CORRESPONDENCE**



## APPENDIX I. INITIAL PLAN FOR PAMS REQUIRED SITES

The Bay Area Air Quality Management District (Air District) voluntarily operated two unofficial Photochemical Assessment Monitoring Stations (PAMS) sites (Livermore and San Ramon) as a PAMS-like network to better understand ozone formation episodes and enhance forecasting capabilities (see Section 5.4 for more details). While a PAMS network was previously required for only serious, severe, or extreme ozone nonattainment areas, the recently revised monitoring rule (80 FR 65292; October 26, 2015) requires PAMS measurements June 1 through August 31 at NCore sites that are located in Core-Based Statistical Areas (CBSAs) with populations of 1,000,000 or more, starting in 2019. The PAMS measurements at this site must include hourly measurements of speciated VOCs, O<sub>3</sub>, NO, true NO<sub>2</sub>, NO<sub>y</sub>, ambient temperature, wind speed, wind direction, atmospheric pressure, relative humidity, precipitation, mixing-height, solar radiation, and UV radiation. In addition, three 8-hour average carbonyl samples in a day are required on a 1 in 3 day schedule. The initial plan for implementing this requirement is to be submitted to EPA for their approval by July 1, 2018 (40 CFR 50.10(a)(10)). USEPA has indicated that it is working on a proposed rule to extend the start date of PAMS measurements and expects that this proposed rule change will be signed by June 1, 2019. As a result of the, delay the BAAQMD will not begin making PAMS measurements at the Livermore (approved NCore-waiver site location) in 2019, and will work with EPA to begin measurements on or before the final revised start date for this network. However, EPA has requested that monitoring agencies submit the following information by July 1, 2017.

### **Network Decision**

- The NCore site located at San Jose – Jackson will serve as the location of the required PAMS site and will measure the following parameters described below. An inventory of equipment used at the site(s) is provided in Attachment 2.
- We request a waiver from implementing PAMS at an otherwise required NCore site entirely, or to make PAMS measurements at alternative locations such as existing PAMS sites or existing NATTS sites. The Air District is requesting approval for an alternate location, the current unofficial-PAMS site in Livermore, per 40 CFR 58 Appendix D 5(c). Rationale for this waiver is provided in Attachment 1. An inventory of equipment the Air District expects to use at the site is provided in Attachment 2.

### **Auto GC Decision**

Volatile organic compounds (VOCs) – Table H-1 includes a draft list of the targeted VOCs not yet finalized by EPA.

- We will measure hourly speciated VOC measurements with an auto-gas chromatograph (GC). An inventory of equipment the Air District expects to use at the site is provided in Attachment 2.
- We request a waiver to allow three 8-hour samples every third day as an alternative to daily hourly speciated VOC measurements at locations (insert locations).

**Meteorology Measurements Decision**

EPA is suggesting the use of ceilometers for determining mixing height, however other types of meteorological equipment that provide for an indication of mixing height can be proposed.

- Will measure wind direction, wind speed, temperature, humidity, atmospheric pressure, precipitation, solar radiation, ultraviolet radiation, and mixing height. An inventory of equipment the Air District expects to use at the site is provided in Attachment 2.
- We request a waiver to allow meteorological measurements to be obtained from other nearby sites.

**Other Required Measurements**

Carbonyls – The Air District intends to meet the carbonyl sampling requirement with continuous formaldehyde sampling if instrumentation that meets performance specifications is identified. The Air District prefers this option due to added value of increased temporal resolution and significant resource savings in operational expenses and staff time. If this option is not technically feasible, the Air District will conduct discrete cartridge sampling using a Xontech 924 or similar instrumentation (has not yet been purchased) and the national contract lab for analyses and data reporting. If selected, cartridge sampling will be conducted at a frequency of three 8-hour samples on a one-in-three day basis. Table H-1 lists the target carbonyls analyzed by the contract lab if the discrete sampling option is chosen (not yet finalized by EPA).

Nitrogen Oxides – The Air District will monitor for NO and NO<sub>y</sub> (total oxides of nitrogen) in addition to true NO<sub>2</sub>. The true NO<sub>2</sub> is required to be measured with a direct reading NO<sub>2</sub> analyzer, cavity attenuated phase shift (CAPS) spectroscopy or photolytic-converter NO<sub>x</sub> analyzer. An inventory of equipment the Air District expects to use at the site is provided in Attachment 2.

**Table H-1. PAMS Target Compound List**

Priority Compounds				Optional Compounds			
1	1,2,3-trimethylbenzene <sup>a</sup>	19	n-hexane <sup>b</sup>	1	1,3,5-trimethylbenzene	19	m-diethylbenzene
2	1,2,4-trimethylbenzene <sup>a</sup>	20	n-pentane	2	1-pentene	20	methylcyclohexane
3	1-butene	21	o-ethyltoluene <sup>a</sup>	3	2,2-dimethylbutane	21	methylcyclopentane
4	2,2,4-trimethylpentane <sup>b</sup>	22	o-xylene <sup>a,b</sup>	4	2,3,4-trimethylpentane	22	n-decane
5	acetaldehyde <sup>b,c</sup>	23	p-ethyltoluene <sup>a</sup>	5	2,3-dimethylbutane	23	n-heptane
6	acetone <sup>c,d</sup>	24	Propane	6	2,3-dimethylpentane	24	n-nonane
7	benzene <sup>a,b</sup>	25	propylene	7	2,4-dimethylpentane	25	n-octane
8	c-2-butene	26	styrene <sup>a,b</sup>	8	2-methylheptane	26	n-propylbenzene <sup>a</sup>
9	ethane <sup>d</sup>	27	toluene <sup>a,b</sup>	9	2-methylhexane	27	n-undecane
10	ethylbenzene <sup>a,b</sup>	28	t-2-butene	10	2-methylpentane	28	p-diethylbenzene
11	Ethylene			11	3-methylheptane	29	t-2-pentene
12	formaldehyde <sup>b,c</sup>			12	3-methylhexane	30	α/β-pinene
13	Isobutane			13	3-methylpentane	31	1,3 butadiene <sup>b</sup>
14	Isopentane			14	Acetylene	32	benzaldehyde <sup>c</sup>
15	Isoprene			15	c-2-pentene	33	carbon tetrachloride <sup>b</sup>
16	m&p-xylenes <sup>a,b</sup>			16	cyclohexane	34	Ethanol
17	m-ethyltoluene <sup>a</sup>			17	cyclopentane	35	Tetrachloroethylene <sup>b</sup>
18	n-butane			18	isopropylbenzene <sup>b</sup>		

Source: Revisions to the Photochemical Assessment Monitoring Stations Compound Target List.  
U.S. EPA, November 20, 2013

<sup>a</sup> Important SOAP (Secondary Organic Aerosols Precursor) Compounds

<sup>b</sup> HAP (Hazardous Air Pollutant) Compounds

<sup>c</sup> Carbonyl compounds

<sup>d</sup> Non-reactive compounds, not considered to be VOC for regulatory purposes

## **Attachment 1: PAMS Required Site Location Waiver Request and Rationale**

The Bay Area Air Quality Management District (Air District) is requesting that EPA approve a waiver to operate the required PAMS site at our current unofficial PAMS location at Livermore (AQS ID 06-001-0007), rather than our NCore site at San Jose – Jackson (AQS ID 06-085-0005). The Livermore site has been the design value site for the Bay Area ozone nonattainment area since 2003-2005. As such, it is the critical site for any required attainment modeling, and therefore it will be more useful to have precursor and meteorological measurements at Livermore than at San Jose – Jackson. Due to the flight path for the San Jose International Airport, meteorological measurements are impossible to conduct at the San Jose – Jackson site, so implementing PAMS at Livermore allows for these measurements at the same location as the O<sub>3</sub> and O<sub>3</sub> precursor measurements, which is also preferable for model validation. Finally, the Air District has conducted O<sub>3</sub> precursor measurements at the Livermore site since 2010, making it a better site to continue to assess trends in the concentrations of these precursors.

**Attachment 2: Current Equipment Plans for the PAMS Required Site**

<b>Parameter</b>	<b>Equipment</b>
VOC	Perkin Elmer TD300 with Clarus GC
True NO <sub>2</sub>	API T500U (CAPS)
NO/NO <sub>y</sub>	API T200 EU/NO <sub>y</sub>
Carbonyls	Continuous formaldehyde sampler or Xontech 924 or similar
Mixing Height	Vaisala CL-51 (ceilometer)
Wind Direction, Wind Speed	Climatronics F460 cup and vane
Ambient Temperature	Campbell Scientific CS107
Relative Humidity	Vaisala HMP-45
Barometric Pressure	Vaisala PTB110
Solar Radiation	Eppley 8-48
UV Radiation	Eppley TUVR
Precipitation	Texas Electronics TR-525USW (tipping bucket)



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY

REGION IX

75 Hawthorne Street

San Francisco, CA 94105-3901

OCT 30 2017

Mr. Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street  
San Francisco, California 94105

Dear Mr. Stevenson:

Thank you for your submission of the Bay Area Air Quality Management District's (BAAQMD's) 2016 *Air Monitoring Network Plan* on June 29, 2017. We have reviewed the submitted document based on the requirements set forth under 40 CFR 58. Based on the information provided in the plan, the U.S. Environmental Protection Agency (EPA) approves all portions of the network plan except those specifically identified below. With this plan approval, we also formally approve the waiver to locate your required PAMS site at Livermore (AQS ID: 06-001-0007) rather than at San Jose-Jackson (AQS ID: 06-085-0005). We are also transmitting approval from the Office of Air Quality Planning and Standards (OAQPS) of your request for a waiver to operate a  $\text{NO}_x$  monitor in lieu of  $\text{NO}_y$  at San Jose-Jackson, in order to locate the  $\text{NO}_y$  monitor at Livermore to support PAMS. More information about these approvals is in Enclosures D and E.

Please note that we cannot approve portions of the annual network plan for which the information in the plan is insufficient to judge whether the requirement has been met, or for which the information, as described, does not meet the requirements as specified in 40 CFR 58.10 and the associated appendices. EPA Region 9 also cannot approve portions of the plan for which the EPA Administrator has not delegated approval authority to the regional offices. Accordingly, the first enclosure (*A. Annual Monitoring Network Plan Items where EPA is Not Taking Action*) provides a listing of specific items of your agency's annual monitoring network plan where EPA is not taking action. The second enclosure (*B. Additional Items Requiring Attention*) is a listing of additional items in the plan that EPA wishes to bring to your agency's attention.

The third enclosure (*C. Annual Monitoring Network Plan Checklist*) is the checklist EPA used to review your plan for overall items that are required to be included in the annual network plan along with our assessment of whether the plan submitted by your agency addresses those requirements. The fourth enclosure (*D. EPA approval of the waiver request to locate PAMS at Livermore*) documents EPA's approval of the request for a waiver to locate your required PAMS site at Livermore rather than at San Jose-Jackson, as requested in Appendix H of your plan. The fifth and final enclosure (*E. EPA approval of an  $\text{NO}_y$  waiver at San Jose-Jackson*) includes a copy of correspondence between EPA Region 9 and EPA OAQPS discussing and granting

approval of a waiver to operate a NO<sub>x</sub> monitor in lieu of NO<sub>y</sub> at San Jose-Jackson, based on the information provided in Appendices F and H and elsewhere in your plan.

The first two enclosures highlight a subset of the more extensive list of items reviewed in the third enclosure. All comments conveyed via this letter (and enclosures) should be addressed (through corrections within the plan, additional information being included, or discussion) in next year's annual monitoring network plan.

If you have any questions regarding this letter or the enclosed comments, please feel free to contact me at (415) 947-4134 or Anna Mebust at (415) 972-3265.

Sincerely,



Gwen Yoshimura, Manager  
Air Quality Analysis Office

Enclosures:

- A. Annual Monitoring Network Plan Items where EPA is Not Taking Action
- B. Additional Items Requiring Attention
- C. Annual Monitoring Network Plan Checklist
- D. EPA approval of the waiver request to locate PAMS at Livermore
- E. EPA correspondence and approval of an NO<sub>y</sub> waiver at San Jose-Jackson

cc (via email): Charley Knoderer, BAAQMD  
Gayle Sweigert, California Air Resources Board (CARB)  
Sunghoon Yoon, CARB  
Ranjit Bhullar, CARB

## **APPENDIX J. SULFUR DIOXIDE DATA REQUIREMENTS RULE COMPLIANCE INFORMATION**

On March 18, 2016, the U.S. Environmental Protection Agency sent a letter to the California Air Resources Board, informing the state that they considered three sources in Martinez, California, to be aggregated with respect to triggering compliance with the sulfur dioxide Data Requirements Rule ambient air characterization requirements. These sources are the Shell and Tesoro refineries and the Eco Services sulfur recovery plant. The Air District prepared an [analysis](#) (see below) outlining the proposed compliance with the sulfur dioxide Data Requirements Rule through ambient air monitoring. The Air District solicited comments from the public on this analysis from September 29 through October 31, 2016, and submitted it to the EPA. The EPA [approved](#) this approach on December 6, 2016 (see below).





**BAY AREA  
AIR QUALITY  
MANAGEMENT  
DISTRICT**

- ALAMEDA COUNTY**  
Tom Bates  
Scott Haggerty  
Rebecca Kaplan  
Nate Miley
- CONTRA COSTA COUNTY**  
John Gioia  
David Hudson  
(Secretary)  
Karen Mitchoff  
Mark Ross
- MARIN COUNTY**  
Katie Rice
- NAPA COUNTY**  
Brad Wagenknecht
- SAN FRANCISCO COUNTY**  
John Avalos  
Edwin M. Lee  
Eric Mar  
(Chair)
- SAN MATEO COUNTY**  
David J. Canepa  
Carole Groom  
Warren Slocum
- SANTA CLARA COUNTY**  
Cindy Chavez  
Liz Kniss  
(Vice-Chair)  
Jan Pepper  
Rod G. Sinks
- SOLANO COUNTY**  
James Spering  
Osby Davis
- SONOMA COUNTY**  
Teresa Barrett  
Shirlee Zane

Jack P. Broadbent  
EXECUTIVE OFFICER/APCO

Connect with the  
Bay Area Air District:



September 29, 2016

Anita Lee, Ph.D.  
Manager, Air Quality Analysis Office  
U.S. EPA Region 9  
75 Hawthorne Street  
San Francisco, CA 94105-3901

RE: 2015 Annual Network Plan

Dear Dr. Lee

On March 18, 2016, EPA sent a letter to the California Air Resources Board, informing the state that they considered three sources in Martinez, California, to be aggregated with respect to triggering compliance with the sulfur dioxide Data Requirements Reporting Rule (SO<sub>2</sub> DRR) ambient air characterization requirements. These sources (the Shell and Tesoro refineries, and the Eco Services sulfur recovery plant) are within the jurisdiction of the Bay Area Air Quality Management District ("Air District").

In our 2015 Annual Monitoring Network Plan, the Air District indicated that we intend to comply with the SO<sub>2</sub> DRR using the existing Martinez SO<sub>2</sub> monitoring station to fulfill the monitoring option. The attached document includes additional information supporting the Air District's approach to rely on the ongoing SO<sub>2</sub> monitoring at the Martinez site to satisfy this requirement for ambient air quality characterization.

This document is currently available for public comment on our website until October 31, 2016. Please contact me at (415) 749-4695 with any questions or concerns.

Sincerely,

Eric D. Stevenson  
Director of Meteorology, Measurement, and Rules

Attachment

cc: Gayle Sweigert, California Air Resources Board

## Analysis of the suitability of the Martinez SO<sub>2</sub> SLAMS to fulfill the monitoring requirement of the SO<sub>2</sub> Data Requirements Rule

The SO<sub>2</sub> Data Requirements Rule (SO<sub>2</sub> DRR), finalized by EPA on August 21, 2015, requires states to characterize ambient sulfur dioxide (SO<sub>2</sub>) concentrations in areas around sources emitting greater than 2000 tons per year (tpy) of SO<sub>2</sub>. The rule includes the flexibility for areas to meet this requirement through ambient air monitoring, modeling, or by the source adopting enforceable limits to bring emissions below 2000 tpy. On March 18, 2016, EPA sent a letter to the California Air Resources Board, informing the state that they considered three sources in Martinez, California, to be aggregated with respect to triggering compliance with the SO<sub>2</sub> DRR ambient air characterization requirements. These facilities and their 2014 calendar year emissions are listed in Table 1, below.

**Table 1: Martinez Facility SO<sub>2</sub> Emissions for Calendar Year 2014**

Facility Name	Source Type	SO <sub>2</sub> (tons/yr)
Shell	Petroleum Refinery	1,093
Eco Services (formerly Solvay)	Sulfuric Acid Plant	186
Tesoro	Petroleum Refinery	962
Aggregated Total	-	2,241

Martinez is situated in a small basin bordered on the north by the Carquinez Strait, connecting the San Pablo and Suisun Bays, and in the other directions by hills that range in height from 200-400 meters. Due to the complicated topography and meteorology of the area surrounding these sources, heavily influenced by sea-breezes and orographic forcing, typical dispersion modeling does not accurately characterize ambient concentrations of pollutants. However, such modeling can be used to help identify areas of relative maximum concentration.

The Bay Area Air Quality Management District (“Air District”) completed 1-hour SO<sub>2</sub> modeling for the Martinez area using the AERMOD dispersion model to evaluate the normalized ambient SO<sub>2</sub> concentrations resulting from the combined SO<sub>2</sub> source emissions from Shell, Tesoro, and Eco Services. The modeling was performed according to the following specifications:

- A 16 km x 16 km special receptor grid containing 16,600 discrete receptor locations centered on UTM: 580,124 E, 4,208,805 N.
- A combined total of 30 sources of SO<sub>2</sub> at Shell, Tesoro and Eco Services were included in the model. Source locations and stack parameters were previously provided by the facilities.
- SO<sub>2</sub> emission rates used in the model were considered to be maximum values.
- Elevations for sources and receptors were taken from the National Elevation Dataset (NED) using 10 meter horizontal resolution data.

- Five consecutive years of meteorological data (2009 – 2013) from a centrally located meteorological station (called Shell East) was used.

Figure 1 below shows an outline of the domain used for the modeling, the fence lines of the included facilities, and nearby SO<sub>2</sub> monitors. The Air District's SO<sub>2</sub> monitors, also known as state or local air monitoring stations (SLAMS) are labeled with the site name and the monitor type. More detailed information about the modeling protocol, including model inputs, are available upon request to the Air District.

As shown in Figure 2 below, based on the five-year modeling period results, the higher normalized 1-hour SO<sub>2</sub> concentrations are expected to occur generally at elevated areas. The resulting maximum normalized 1-hour SO<sub>2</sub> concentration is about 0.5 km southwest of the existing Air District SO<sub>2</sub> SLAMS. Access to power is very limited in this sparsely populated hilly area, similar to many of the elevated areas surrounding Martinez. Therefore, the Martinez SLAMS current location is likely the closest feasible location to the modeled concentration maximum, given power and siting constraints, as well as being representative of the actual population exposure of the likely maximum 1-hour SO<sub>2</sub> concentrations.

Given the complexity of the area and the resulting challenges in modeling, the Air District performed two additional 5-year modeling runs using the same parameters, but meteorological data from two other nearby meteorological stations (Shell-West, and Tesoro). These runs show other areas of potential high SO<sub>2</sub> concentrations in addition to the consistent high concentration location uphill from the current monitoring SLAMS (see Figures 3 and 4 below). The Air District believes that the varied modeling results support the current monitoring location as adequate to satisfy the monitoring requirement for the SO<sub>2</sub> DRR for the sources EPA identified, however, the Air District will continue to evaluate the appropriateness of this location to meet this objective in each 5-year network assessment. Any such assessment will utilize new information that may become available, such as data from upcoming community monitoring sites. In the next few years, the Air District expects to install monitors in the communities surrounding the five Bay Area refineries to further characterize the air quality near those sources as required by our Regulation 3.

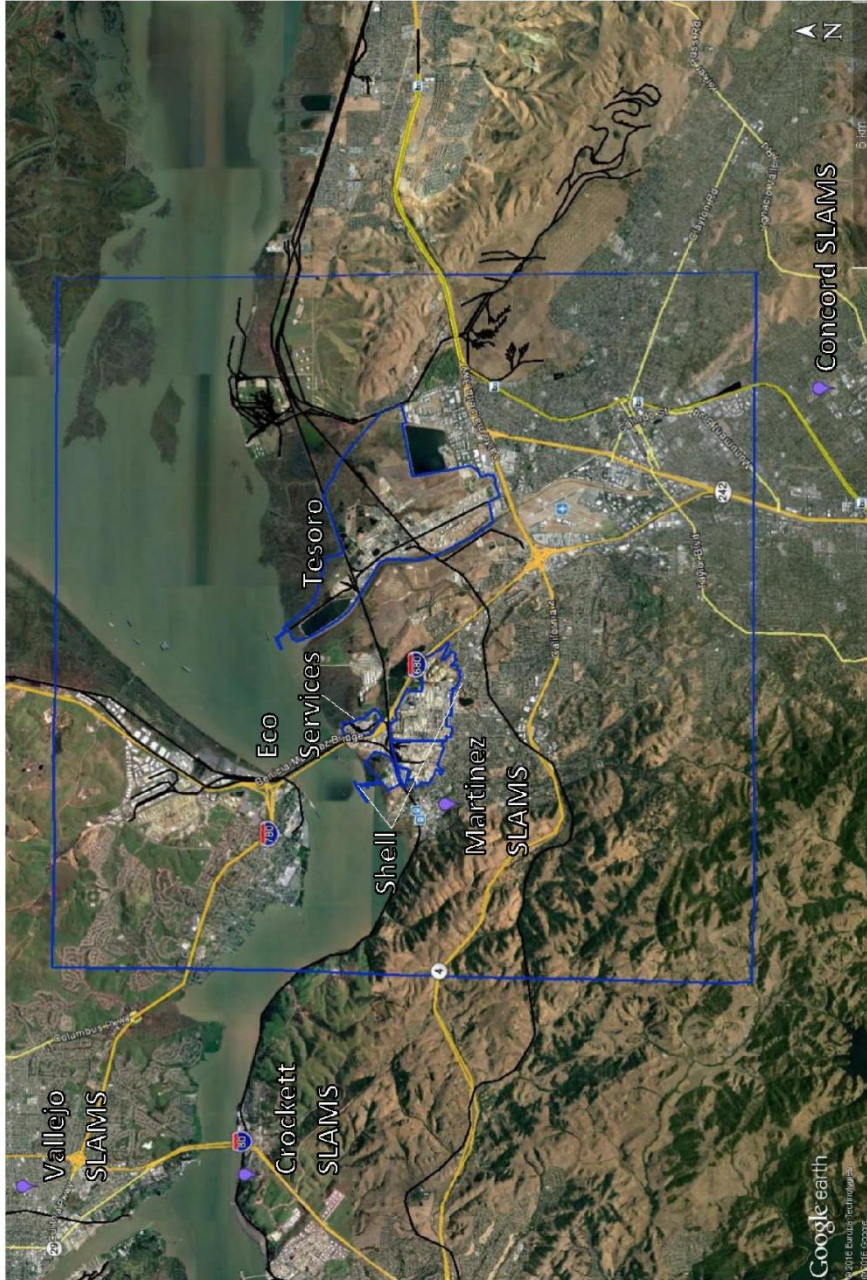


Figure 1: Area overview including the AERMOD modeling domain (blue rectangle), facilities subject to the SO<sub>2</sub> DRB, and nearby SO<sub>2</sub> monitoring sites



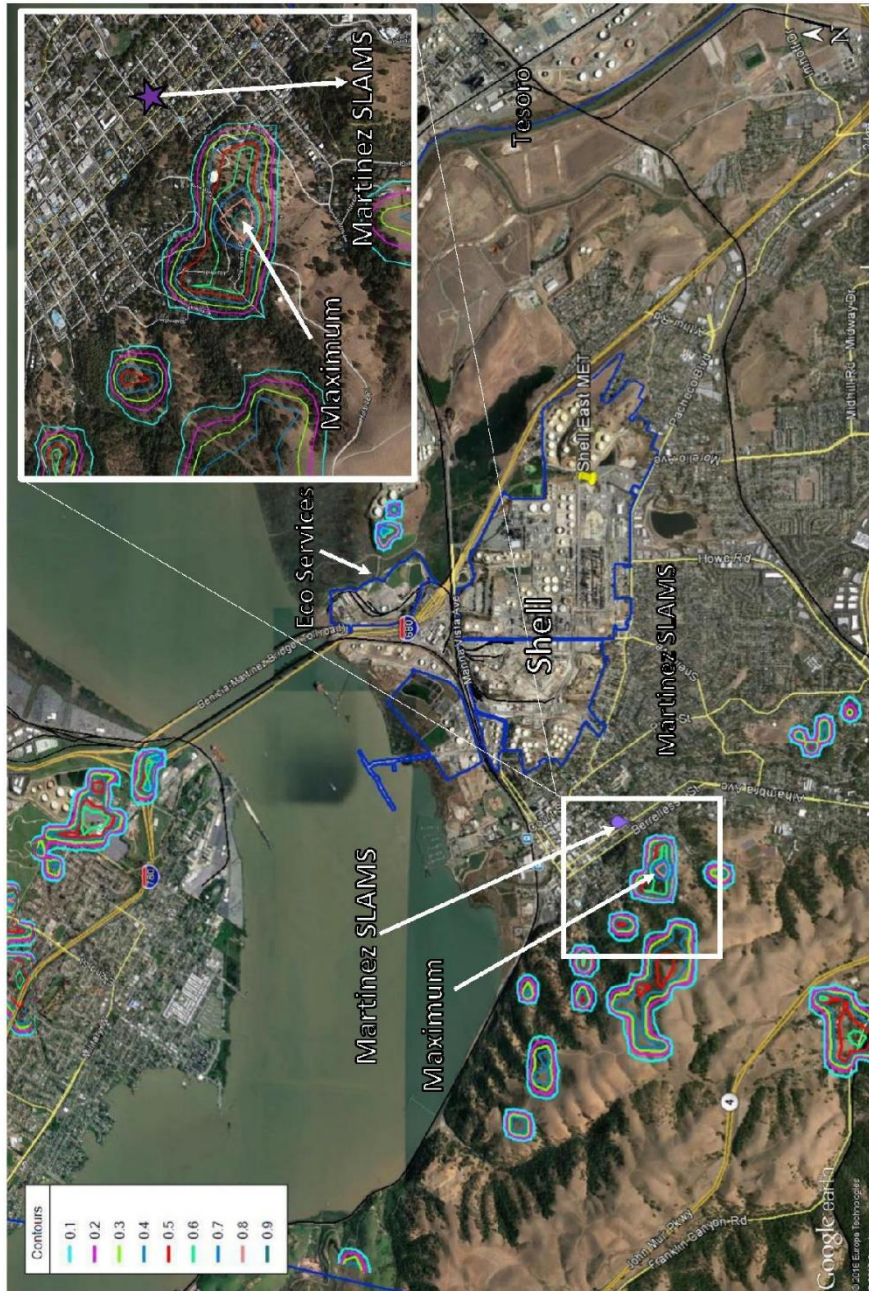


Figure 2: Maximum normalized 1-hour SO2 concentrations from AERMOD modeling using emissions from Shell, Tesoro, and Eco Services, and 2009-2013 Shell-East meteorological data



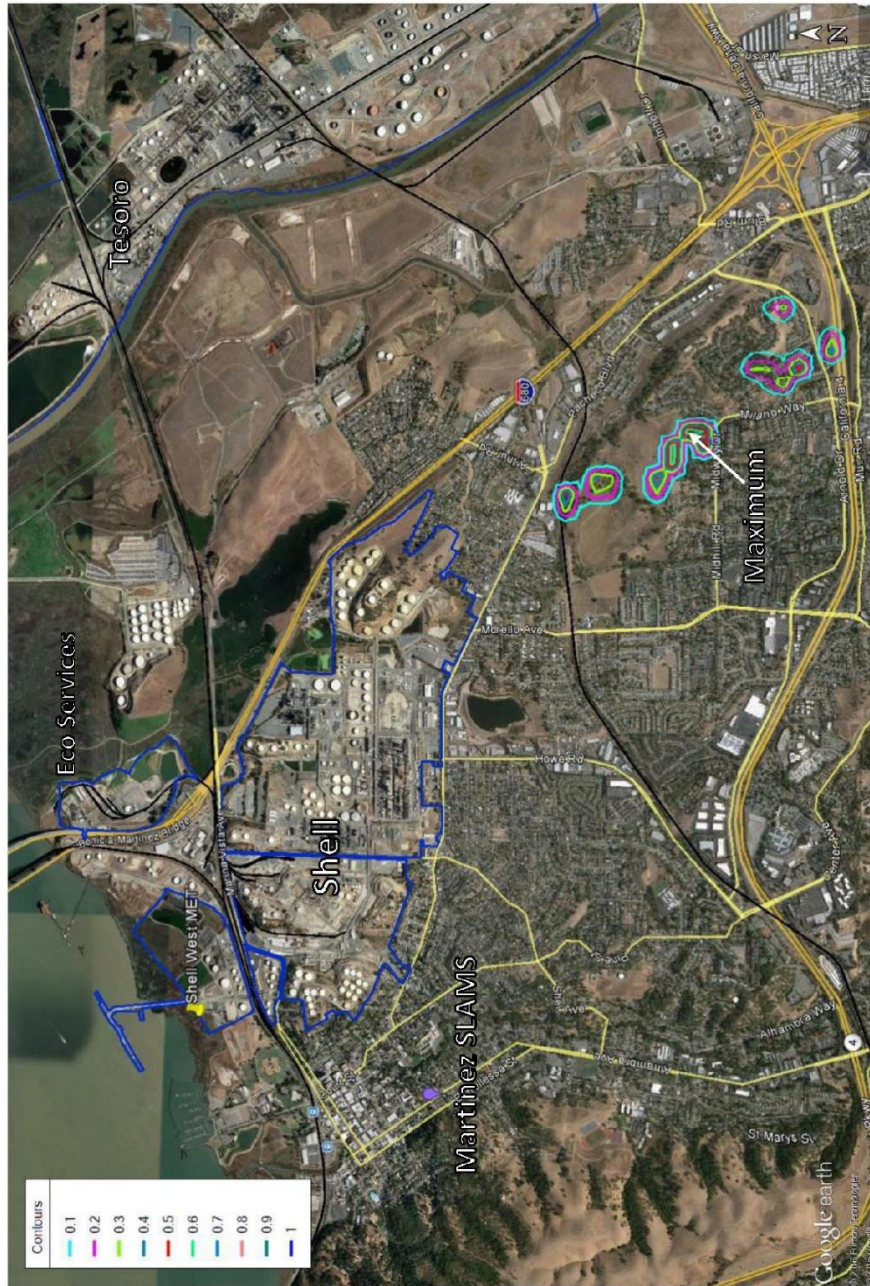


Figure 3: Maximum normalized 1-hour SO2 concentrations from AERMOD modeling using emissions from Shell, Tesoro, and Eco Services, and 2009-2013 Shell-West meteorological data



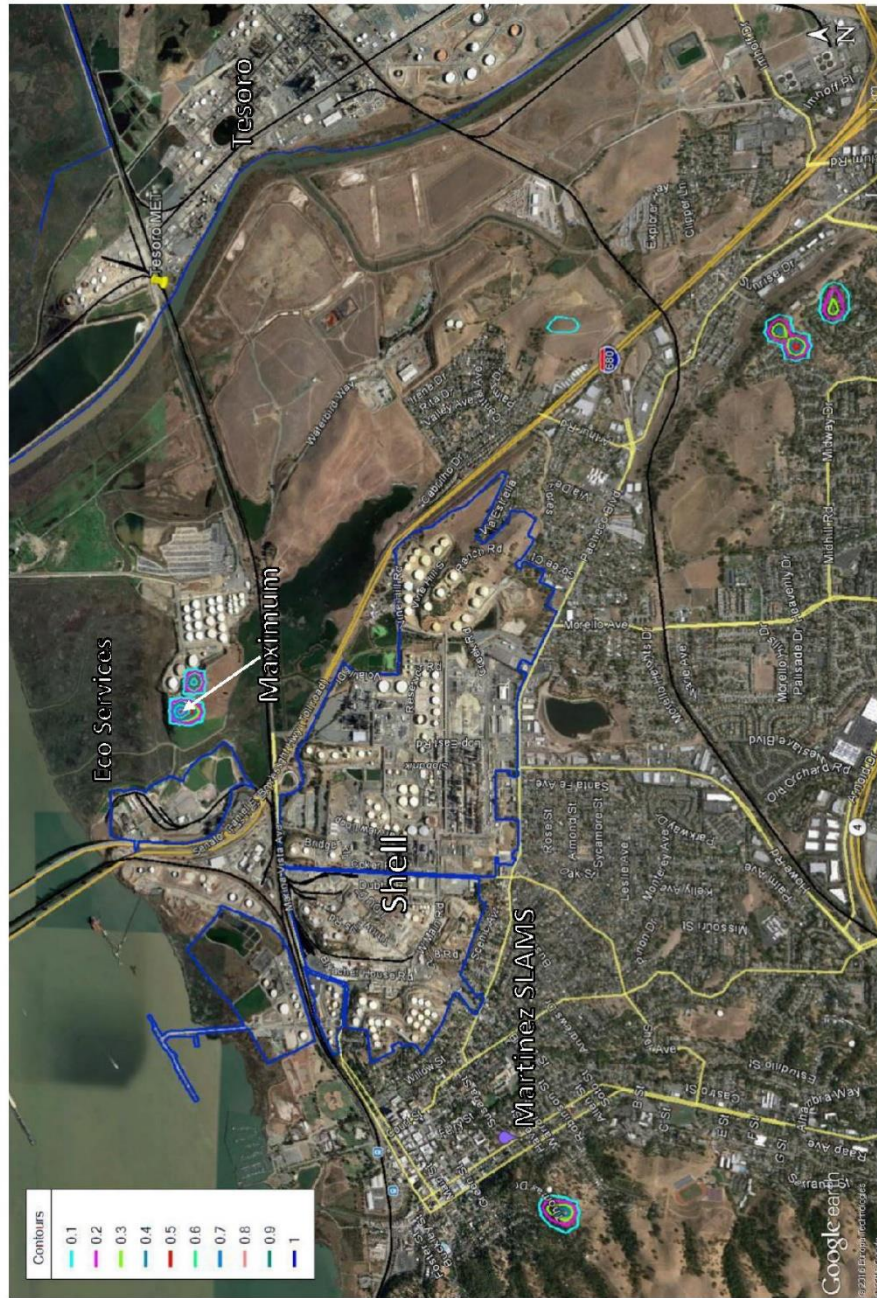


Figure 4: Maximum normalized 1-hour SO<sub>2</sub> concentrations from AERMOD modeling using emissions from Shell, Tesoro, and Eco Services, and 2009-2013 Tesoro meteorological data



UNITED STATES ENVIRONMENTAL PROTECTION AGENCY  
REGION IX  
75 Hawthorne Street  
San Francisco, CA 94105

December 6, 2016

Mr. Eric Stevenson  
Director of Technical Services  
Bay Area Air Quality Management District  
375 Beale Street  
San Francisco, California 94105

Dear Mr. Stevenson:

Thank you for your September 29, 2016 submission of your analysis of the suitability of the Martinez SO<sub>2</sub> State or Local Air Monitoring Station (SLAMS) to fulfill the monitoring requirement of the SO<sub>2</sub> Data Requirements Rule, as well as the October 5, 2016 submission of the Interoffice Memorandum describing the modeling protocol and source parameter data used in the analysis. The analysis was made available for public comment between September 29, 2016 and October 31, 2016. In your 2015 Air Monitoring Network Plan, submitted June 27, 2016, you described your intent to perform this analysis and submit it to EPA. We approved your network plan on October 31, 2016, and included a comment in Enclosure C, checklist item 63, stating that "...BAAQMD and EPA are currently evaluating whether existing SO<sub>2</sub> monitoring is adequate to meet the requirements of DRR."

On December 5, 2016 your staff communicated to us via email that no comments on the analysis were received. Based on the information we received from your agency, we approve the current location of the Martinez SO<sub>2</sub> SLAMS to satisfy monitoring requirements under the SO<sub>2</sub> Data Requirements Rule.

If you have any questions regarding this letter, please feel free to contact me at (415) 947-4134 or Anna Mebust at (415) 972-3265.

Sincerely,

A handwritten signature in blue ink, appearing to read "Gwen Yoshimura".

Gwen Yoshimura, Acting Manager  
Air Quality Analysis Office

cc (via email): Katherine Hoag, Bay Area Air Quality Management District  
Gayle Sweigert, California Air Resources Board